

## Soft, flexible and transparent graphene-based active spinal cord implants for optogenetic studies

Velea, A.; Vollebregt, S.; Giagka, Vasiliki

### Publication date

2020

### Document Version

Final published version

### Citation (APA)

Velea, A., Vollebregt, S., & Giagka, V. (2020). *Soft, flexible and transparent graphene-based active spinal cord implants for optogenetic studies*. Poster session presented at 13th International Symposium on Flexible Organic Electronics (ISFOE20), Thessaloniki, Greece.

### Important note

To cite this publication, please use the final published version (if applicable). Please check the document version above.

### Copyright

Other than for strictly personal use, it is not permitted to download, forward or distribute the text or part of it, without the consent of the author(s) and/or copyright holder(s), unless the work is under an open content license such as Creative Commons.

### Takedown policy

Please contact us and provide details if you believe this document breaches copyrights. We will remove access to the work immediately and investigate your claim.

## Soft, flexible and transparent graphene-based active spinal cord implants for optogenetic studies

A. I. Velea<sup>1,2,3</sup>, S. Vollebregt<sup>2</sup>, V. Giagka<sup>1,3</sup>

<sup>1</sup>Bioelectronics Section and <sup>2</sup>Electronic Components, Technology and Materials section, Department of Microelectronics, Faculty of Electrical Engineering, Mathematics and Computer Science, Delft University of Technology  
Mekelweg 4, 2628 CD, Delft, The Netherlands

<sup>3</sup>Technologies for Bioelectronics Group, Department of System Integration and Interconnection Technologies, Fraunhofer Institute for Reliability and Microintegration IZM  
Gustav-Meyer-Allee 25, 13355, Berlin, Germany  
e-mail: a.velea-1@tudelft.nl; andrada.iulia.velea@izm.fraunhofer.de

Patients affected by spinal cord injuries (SCI) are usually unable to perform trivial motor activities and thus, for therapeutic purposes, epidural spinal cord stimulation (ESCS) is currently used. Moreover, more exploratory research, using optogenetics, is being conducted in rodents for a better understanding of the mechanisms that occur while delivering specific therapies. However, the availability of tailored neurotechnologies for such experiments is limited.

This work reports the development and characterization of flexible, active spinal cord implants with optogenetic compatibility<sup>1,2</sup> (Fig.1). A scalable and reproducible microfabrication process has been developed, using graphene<sup>3</sup>, a transparent, flexible and conductive material, to form the electrodes and interconnects of the implant. Small and thin<sup>4</sup> electronic chips were assembled via flip-chip bonding processes either on graphene or on metal-on-graphene layers. Soft, polymeric encapsulation was employed to sustain the high flexibility and transparency of the implant. The result is an active prototype consisting of a multi-layered graphene structure between two polymeric-based encapsulation layers, with thin chips integrated on the implant and test pads for interconnection to the outside world.

Raman spectroscopy and optical transmittance were employed for the characterization of the graphene layer while cyclic voltammetry and electrochemical impedance spectroscopy were performed to benchmark the electrical properties of the device. The assembly process of the chips was evaluated using four-point electrical measurements.

In this work, the first transparent, graphene-based active implants have been developed (Fig. 2 and Fig. 3). The prototypes were extensively characterized and the results showed a transparency of ~80 % as well as no deterioration over time when soaked in saline solution or when bent under various angles. The graphene electrodes showed an impedance of ~8 k $\Omega$  at 1 kHz frequencies and the resistance after the bonding process ranged from 10 m $\Omega$  up to 16  $\Omega$  for individual connections, depending on the substrate used.

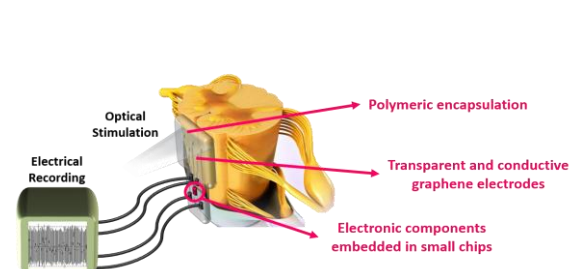


Fig. 1. Envisioned structure of the proposed system

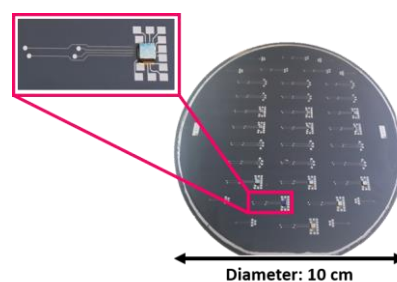


Fig. 2. Active prototypes developed on a silicon wafer

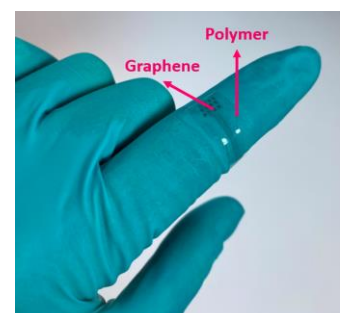


Fig. 3. Soft, flexible, graphene-based implants

1. A. I. Velea, S. Vollebregt, G. K. Wardhana, and V. Giagka, "Wafer-scale graphene-based soft implant with optogenetic compatibility," in Proc. *IEEE MEMS 2020*, Vancouver, Canada, Jan. 2020.
2. A. I. Velea, S. Vollebregt, Tim Hosman, A. Pak, and V. Giagka, "Towards a Microfabricated Flexible Graphene-Based Active Implant for Tissue Monitoring During Optogenetic Spinal Cord Stimulation," in Proc. *IEEE Nanotech. Mater. Dev. Conf. (NMDC) 2019*, Stockholm, Sweden, Oct. 2019.
3. S. Vollebregt et al., "A transfer-free wafer-scale CVD graphene fabrication process for MEMS/NEMS sensors", in Proc. *IEEE MEMS 2016*, pp.17 – 20, Shanghai, China, Jan. 2016.
4. V. Giagka, N. Saeidi, A. Demosthenous, and N. Donaldson, "Controlled silicon IC thinning on individual die level for active implant integration using a purely mechanical process," in Proc. *ECTC 2014*, Orlando, FL, USA, May 2014, pp. 2213 – 2219.