

Current Challenges in Ultrasound Imaging of Cortical Bone Thickness

Renaud, Guillaume; Minonzio, Jean Gabriel

DOI

[10.1016/j.acra.2023.08.043](https://doi.org/10.1016/j.acra.2023.08.043)

Publication date

2023

Document Version

Final published version

Published in

Academic Radiology

Citation (APA)

Renaud, G., & Minonzio, J. G. (2023). Current Challenges in Ultrasound Imaging of Cortical Bone Thickness. *Academic Radiology*, 30(12), 3162-3164. <https://doi.org/10.1016/j.acra.2023.08.043>

Important note

To cite this publication, please use the final published version (if applicable). Please check the document version above.

Copyright

Other than for strictly personal use, it is not permitted to download, forward or distribute the text or part of it, without the consent of the author(s) and/or copyright holder(s), unless the work is under an open content license such as Creative Commons.

Takedown policy

Please contact us and provide details if you believe this document breaches copyrights. We will remove access to the work immediately and investigate your claim.



Current Challenges in Ultrasound Imaging of Cortical Bone Thickness

Guillaume Renaud, Jean-Gabriel Minonzio

The recent article by Gokcek et al. (1) reported an increased cortical thickness associated with osteoporosis at the ultradistal radius and tibia using conventional ultrasound imaging. This result contradicts a large body of work, including ex vivo and in vivo studies. In particular, numerous studies with high-resolution peripheral quantitative computed tomography (HR-pQCT) have shown that the cortical thickness at the distal radius and at the distal tibia decreases with osteoporosis (2–7). In our opinion, the study by Gokcek et al. (1) holds two severe flaws:

- 1) Current clinical ultrasound scanners are incapable of recovering an accurate and sharp image of the bone cortex.
- 2) The “echo length” from the ultradistal outer bone surface in the ultrasound image is not the cortical thickness.

CURRENT CLINICAL ULTRASOUND SCANNERS ARE INCAPABLE OF RECOVERING AN ACCURATE AND SHARP IMAGE OF THE BONE CORTEX

The authors of (1) cited our work (8), where we demonstrated that advanced ultrasound image reconstruction can recover the accurate cortical thickness at the diaphysis of long bones. Our approach enables the correction of (1) refraction as ultrasound enters or exits the bone cortex since the ultrasound wave speed in cortical bone is typically more than twice larger than that in soft tissues surrounding the cortex and (2) ultrasound wave speed anisotropy in cortical bone since the organized microstructure of cortical bone tissue causes direction-dependent ultrasound wave speed.

However, such advanced ultrasound image reconstruction is not yet available on clinical ultrasound scanners. Until now, clinical ultrasound scanners have been dedicated to soft tissue imaging, assuming the scanned region is made of a uniform soft-tissue medium during image reconstruction. Thus, current clinical ultrasound scanners are incapable of reconstructing an accurate and sharp image inside the bone cortex and hence incapable of evaluating the cortex thickness because they do not take into account the complex ultrasound physics in cortical bone.

THE “ECHO LENGTH” FROM THE ULTRADISTAL OUTER BONE SURFACE IN THE ULTRASOUND IMAGE IS NOT THE CORTICAL THICKNESS

The authors in (1) used the apparent “echo length” of the ultrasound echo generated by the reflection at outer surface of the bone cortex to evaluate the cortical bone thickness. However, the apparent “echo length” is not the cortical thickness, and it depends on multiple factors:

- i. The method chosen to determine the echo length, i.e., how is the beginning and the end of the echo defined, as well as the display settings chosen on the ultrasound scanner (gain, dynamic range...)
- ii. The spatial resolution provided by the ultrasound transducer
- iii. The cortical thickness

The method used to measure the “echo length” of the reflection at outer surface of the cortex is poorly described in (1), as the authors only wrote, “*The outer and the inner start and end locations of the first and the most echogenic linear line of the bone cortex in the relevant region were measured perpendicular to the relevant bone cortex axis by optimal focus and zoom adjustment on B-Mode US images*” (page 517 in (1)). The value obtained with this subjective approach depends on the display settings chosen on the ultrasound scanner. A criterion to calculate the apparent echo length must be defined and would likely require postprocessing of the images using a dedicated algorithm and software.

Acad Radiol 2023; 30:3162–3164

From the Department of Imaging Physics, Delft University of Technology, Delft, The Netherlands (G.R.); Escuela de Ingeniería Informática, Centro de Investigación y Desarrollo en Ingeniería en Salud, Universidad de Valparaíso, Valparaíso, Chile (J-G. M.). Received April 17, 2023; revised May 8, 2023; accepted August 30, 2023. Address correspondence to: G.R. e-mail: g.g.j.renaud@tudelft.nl

© 2023 The Association of University Radiologists. Published by Elsevier Inc. All rights reserved.

<https://doi.org/10.1016/j.acra.2023.08.043>

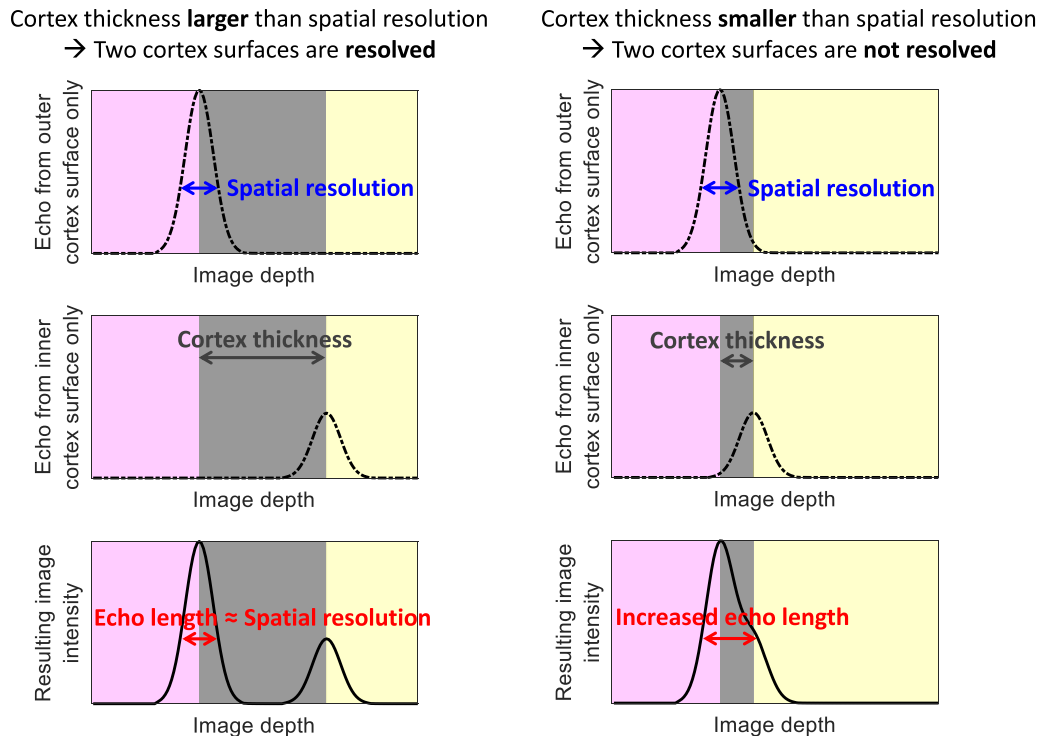


Figure 1. Influence of the cortical thickness and the spatial resolution on the apparent echo length from the outer bone surface in the ultrasound image. Left: case where the inner and outer surfaces of the bone cortex are resolved. Right: case where the cortex surfaces are not resolved.

Thickness measurement or distance measurement between two *resolved* interfaces is reliably performed with ultrasound imaging, for instance, in obstetrics, to evaluate normal fetal growth. Two neighboring interfaces are *resolved* in the ultrasound image if the distance separating them is larger than the spatial resolution in the ultrasound image (Fig 1, left column). In their study, Gokcek et al. (1) used an ultrasound probe that transmits a short ultrasound wavelet with a central frequency close to 7.5 MHz (L12-3E; Mindray Medical International). This probe provides a spatial resolution close to 0.4 mm in cortical bone. If the cortical thickness is larger than 0.4 mm, the outer and the inner surfaces of the bone cortex are resolved and appear as two bright lines in the ultrasound image (Fig. 8 and 9 in (8) and Fig 1, left column). Conversely, if the cortical thickness is smaller than 0.4 mm, the outer and the inner surfaces of the bone cortex are not resolved because the echoes from the two surfaces overlap (Fig 1, right column). As a result, a single bright line appears in the ultrasound image that may be thicker than the spatial resolution.

It is also important to be aware that the relationship between the apparent echo length and the cortical thickness is not monotonic. As illustrated in Figure 2, the apparent echo length shows a maximum value if the cortical thickness is close to the spatial resolution. However, the apparent echo length is smaller and approaches the spatial resolution if the cortical thickness is larger or smaller than the spatial resolution.

Numerous studies with HR-pQCT have reported the cortical thickness at the ultradistal radius (9.5 mm away from

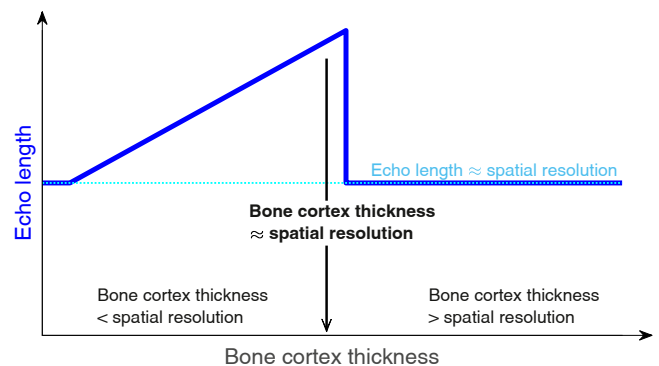


Figure 2. Nonmonotonic relationship between the apparent echo length and the bone cortex thickness.

the joint) and at the ultradistal tibia (22.5 mm away from the joint) (2–7). The ultradistal tibial cortical thickness is slightly larger than that at the ultradistal radius (4). The ultradistal cortical thickness is close to 1 mm in young healthy individuals, and it can become thinner than 0.5 mm in elderly osteoporotic subjects (9). In (1), the authors reported an “echo length” of 0.5 mm in normal individuals and close to 0.6 mm in osteoporotic subjects. The “echo length” of 0.5 mm in normal individuals is thus about twice as smaller than the expected cortical thickness because the “echo length” is unrelated to the cortical thickness and solely determined by the method chosen by the authors to estimate

the “echo length” in the image. The apparent increase in “echo length” from the outer bone surface in osteoporotic subjects is very likely caused by the overlapping of the echoes from the outer and inner surfaces of the bone cortex when the true cortical thickness is smaller or close to the spatial resolution in cortical bone (about 0.4 mm with the ultrasound transducer used in (1)).

The use of the apparent “echo length,” as proposed in (1), could potentially be an interesting clinical parameter for bone health assessment, because simple. However, it is crucial to understand that the apparent “echo length” depends on multiple factors and that the relationship between the apparent “echo length” and the cortical thickness is not monotonic. And most importantly, the echo length should not be confused with the true cortical bone thickness.

DECLARATION OF COMPETING INTEREST

G.R. has patent for Method For Characterising Bone Using Ultrasonic Waves issued to Sorbonne University/Centre National de la Recherche Scientifique/Institut National de la Sante et de la Recherche Medicale/Ecole Superieure de Physique et de Chimie Industrielles de la Ville de Paris.

REFERENCES

1. Gokcek A, et al. Can ultrasonographic measurement of bone cortical thickness predict osteoporosis? *Acad Radiol* 2023; 30(3):516–527.
2. Burghardt AJ, et al. Reproducibility of direct quantitative measures of cortical bone microarchitecture of the distal radius and tibia by HR-pQCT. *Bone* 2010; 47(3):519–528.
3. de Waard EAC, et al. Reliability of HR-pQCT derived cortical bone structural parameters when using uncorrected instead of corrected automatically generated endocortical contours in a cross-sectional study: the Maastricht Study. *Calcif Tissue Int* 2018; 103(3):252–265.
4. Kawalilak CE, et al. Characterizing microarchitectural changes at the distal radius and tibia in postmenopausal women using HR-pQCT. *Osteopor Int* 2014; 25(8):2057–2066.
5. Nishiyama KK, et al. Postmenopausal women with osteopenia have higher cortical porosity and thinner cortices at the distal radius and tibia than women with normal aBMD: an in vivo HR-pQCT study. *J Bone Miner Res* 2010; 25(4):882–890.
6. Vico L, et al. High-resolution pQCT analysis at the distal radius and tibia discriminates patients with recent wrist and femoral neck fractures. *J Bone Miner Res* 2008; 23(11):1741–1750.
7. Zhou B, et al. High-resolution peripheral quantitative computed tomography (HR-pQCT) can assess microstructural and biomechanical properties of both human distal radius and tibia: ex vivo computational and experimental validations. *Bone* 2016; 86:58–67.
8. Renaud G, et al. In vivo ultrasound imaging of the bone cortex. *Phys Med Biol* 2018; 63(12):125010.
9. Krause M, et al. Accuracy of trabecular structure by HR-pQCT compared to gold standard μ CT in the radius and tibia of patients with osteoporosis and long-term bisphosphonate therapy. *Osteopor Int* 2014; 25(5):1595–1606.