

Quantitative fluid dynamic characterization of an organ-on-chip model using phase resolved Doppler OCT

Tugberk, Devrim ; Ballal, Anish; Quirōs-Solano, William ; Speets, P.N.A.; Gaio, N.; Kalkman, J.

Publication date

2023

Document Version

Final published version

Citation (APA)

Tugberk, D., Ballal, A., Quirōs-Solano, W., Speets, P. N. A., Gaio, N., & Kalkman, J. (2023). *Quantitative fluid dynamic characterization of an organ-on-chip model using phase resolved Doppler OCT*. 103-103. Abstract from 2nd Microphysiological Systems World Summit 2023, Berlin, Germany.

Important note

To cite this publication, please use the final published version (if applicable). Please check the document version above.

Copyright

Other than for strictly personal use, it is not permitted to download, forward or distribute the text or part of it, without the consent of the author(s) and/or copyright holder(s), unless the work is under an open content license such as Creative Commons.

Takedown policy

Please contact us and provide details if you believe this document breaches copyrights. We will remove access to the work immediately and investigate your claim.




Abstracts of the 2nd Microphysiological Systems World Summit, Berlin, 2023

Volume 11, No. 1
ISSN 2194-0479
doi:10.58847/ap.2301 (2023)

ALTEX Proceedings

Marcel Leist, Uwe Marx
and Peter Loskill
Welcome

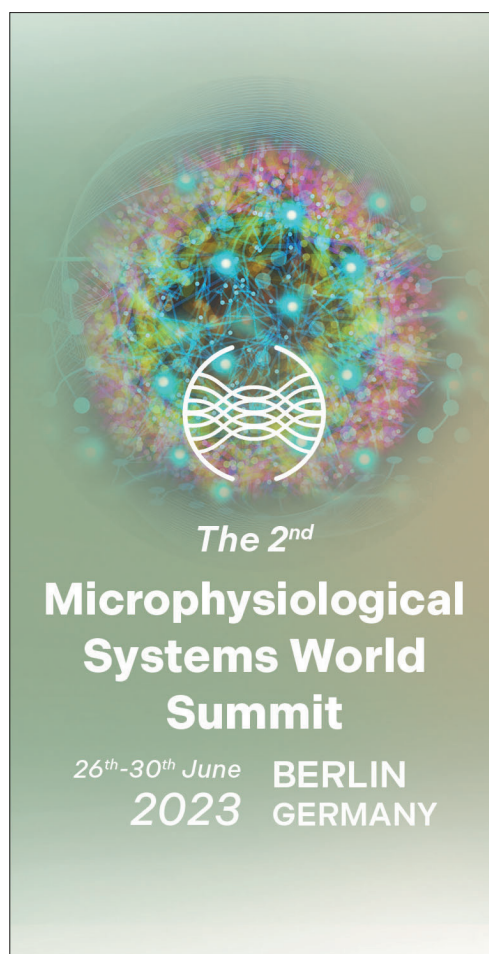

Track 1:
**MPS Development:
Bioengineering Models
and Readouts**

Track 2:
**MPS for Industrial and
Regulatory Application:
Standardization,
QA, Parallelisation and
Automation**

Track 3:
**MPS for Disease
Modelling, Safety Testing
and Basic Research**

Track 4:
**MPS Highlights Across
Disciplines**



compounds, demonstrating its potential to predict safety-related issues before entering the animal testing phase.

References

- [1] Mullard, A. (2016). Parsing clinical success rates. *Nat Rev Drug Discov* 15, 447. doi:10.1038/nrd.2016.136
- [2] Baudy, A. R. et al. (2020). Liver microphysiological systems development guidelines for safety risk assessment in the pharmaceutical industry. *Lab Chip* 20, 215-225. doi:10.1039/c9lc00768g

Presentation: Poster

191

Quantitative fluid dynamic characterization of an organ-on-chip model using phase resolved Doppler OCT

Devrim Tugberk¹, Anish Ballal², William Quirós-Solano³, Peter Speets¹, Nikolas Gaio¹ and Jeroen Kalkman¹

¹TU Delft, Delft, The Netherlands; ²BIOND Solutions, Delft, The Netherlands; ³University of Costa Rica, San Pedro, Costa Rica

a.ballal@biondteam.com

Organ-on-chip (OoC) systems are novel microfluidic microsystems that combine the advantages of well-characterised human cells with the benefits of engineered, physiological-like microenvironments manufactured in the system. The extracellular matrix (ECM) is the natural microenvironment of cells in the human body responsible for providing the appropriate stimuli to cells to control cell processes such as proliferation, migration, and apoptosis. OoCs can mimic the ECM, via channels and porous membranes, by providing the cells with physiological-like mechanical stimuli governed by the fluid dynamics in the system [1]. Understanding the fluid dynamics in OOC can aid in fine-tuning the stimuli sensed by the cultured cells, understanding cell behavior and cell fate. The current state of the art methods for characterizing fluid dynamics in the OoC systems are simulations, theoretical calculations, and empirical observations, therefore a quantitative characterization technique is lacking. Optical coherence tomography (OCT) has been used in previous studies to measure omnidirectional flow velocities in flow systems [2].

In this study, we measured the flow in a cuvette using a Thorlabs GANYMEDE II HR series (high axial resolution of 3 mm in air) spectral domain OCT system. We made quantitative 2D flow measurements using the phase-resolved Doppler method. This work was then extended to extract flow dynamics, in the Bi/ond inCHIPit using titania scattering nanoparticles, which would be a novel way of flow characterization in the field of OOC. The results are compared to the theoretical Hagen-Poiseuille equations and COMSOL simulations and found to be in good agreement. The

results of the study were further extended to determine the shear stress experienced by the cells in the culture well of the OoC.

References

- [1] Menéndez, A. B. C., Du, Z., van den Bosch, T. P. P. et al. (2022). Creating a kidney organoid-vasculature interaction model using a novel organ-on-chip system. *Sci Rep* 12, 1-11. doi:10.1038/s41598-022-24945-5
- [2] Cheishvili, K. and Kalkman, J. (2022). Scanning dynamic light scattering optical coherence tomography for measurement of high omnidirectional flow velocities. *Optics Express* 30, 23382. doi:10.1364/OE.456139

Presentation: Poster

192

Automated and high-volume wafer-scale microfabrication of organ-on-chip (OoC) polymer structures and components

Tawab Karim¹, Nikolas Gaio¹, Sebastiaan Kersjes², Milica Dostanic³ and Massimo Mastrangeli³

¹BIOND Solutions BV, Delft, The Netherlands; ²BESI The Netherlands BV, Duiven, The Netherlands; ³TU Delft, Delft, The Netherlands

t.karim@biondteam.com

Organ-on-chip (OoC) technology is a promising improvement within *in vitro* cell culture, better mimicking functional units of human organs compared to conventional techniques. Current fabrication of three-Dimensional (3D) components in OoC, such as thin membranes and microfluidic structures, is often achieved via soft lithography, bonding, and punching of access holes of polymers, such as polymethylsiloxane (PDMS). However, these methods often suffer from the need of manual fabrication steps, drastically increasing production time and reducing yield due to handling errors and manual alignment of the layers. Consequently, the scalability is limited, which is a crucial aspect for a more widespread adaptation of OoC technology. In this work, we present a reproducible and scalable process for the direct patterning of various 3D polymer structures. The investigated process employs commercially available systems from IC packaging to mould pillars, membranes, and microfluidic channels with varying dimensions and thicknesses. Our process simultaneously improves the control over the thickness and dimensions of these structures in comparison to conventional fabrication techniques. Furthermore, proof of functionality is presented by adapting this technology to an existing OoC platform which incorporates integrated electrodes used for electrophysiological recording, stimulation, and TEER measurements. We demonstrate a complete process for wafer-scale microfabrication of OoCs, enabling low-cost, high-volume automated production. This is an important next step to large-scale manufacturing of