

## Comparing in vivo and ex vivo fiberoptic diffuse reflectance spectroscopy in colorectal cancer

Baltussen, Elisabeth J.M.; Brouwer de Koning, Susan G.; Hendriks, Benno; Józwiak, Katarzyna; Sterenborg, Henricus J.C.M.; Ruers, Theo J.M.

**DOI**

[10.1002/tbio.201900008](https://doi.org/10.1002/tbio.201900008)

**Publication date**

2019

**Document Version**

Final published version

**Published in**

Translational Biophotonics

**Citation (APA)**

Baltussen, E. J. M., Brouwer de Koning, S. G., Hendriks, B., Józwiak, K., Sterenborg, H. J. C. M., & Ruers, T. J. M. (2019). Comparing in vivo and ex vivo fiberoptic diffuse reflectance spectroscopy in colorectal cancer. *Translational Biophotonics*, 1(1-2), Article e201900008. <https://doi.org/10.1002/tbio.201900008>

**Important note**

To cite this publication, please use the final published version (if applicable).  
Please check the document version above.

**Copyright**

Other than for strictly personal use, it is not permitted to download, forward or distribute the text or part of it, without the consent of the author(s) and/or copyright holder(s), unless the work is under an open content license such as Creative Commons.

**Takedown policy**

Please contact us and provide details if you believe this document breaches copyrights.  
We will remove access to the work immediately and investigate your claim.

## FULL ARTICLE

# Comparing in vivo and ex vivo fiberoptic diffuse reflectance spectroscopy in colorectal cancer

Elisabeth J.M. Baltussen<sup>1</sup>  | Susan G. Brouwer De Koning<sup>1</sup> | Benno H.W. Hendriks<sup>2,3</sup> | Katarzyna Józwiak<sup>1,6</sup> | Henricus J.C.M. Sterenberg<sup>1,4</sup> | Theo J.M. Ruers<sup>1,5</sup>

<sup>1</sup>The Netherlands Cancer Institute, Amsterdam, The Netherlands

<sup>2</sup>Philips Research, Eindhoven, The Netherlands

<sup>3</sup>Delft University of Technology, Delft, The Netherlands

<sup>4</sup>Amsterdam University Medical Centre, Amsterdam, The Netherlands

<sup>5</sup>University of Twente, Enschede, The Netherlands

<sup>6</sup>Institute of Biostatistics and Registry Research, Brandenburg Medical School Theodor Fontane, Neuruppin, Germany

## Correspondence

Elisabeth J.M. Baltussen, The Netherlands Cancer Institute, Plesmanlaan 121, 1066 CX Amsterdam, The Netherlands.  
Email: l.baltussen@nki.nl

## Funding information

KWF Kankerbestrijding, Grant/Award Number: NKI 2014-6596; Philips

## Abstract

In vivo data acquisition using fiberoptic diffuse reflectance spectroscopy (DRS) is more complicated and less controlled compared to ex vivo data acquisition. It would be of great benefit if classifiers for in vivo tissue discrimination based on DRS could be trained on data obtained ex vivo. In this study, in vivo and ex vivo DRS

measurements are obtained during colorectal cancer surgery. A mixed model statistical analysis is used to examine the differences between the two datasets. Furthermore, classifiers are trained and tested using in vivo and ex vivo data. It is found that with a classifier trained on ex vivo data and tested on in vivo data, similar results are obtained compared to a classifier trained and tested on in vivo data. In conclusion, under the conditions used in this study, classifiers intended for in vivo tissue discrimination can be trained on ex vivo data.

## KEYWORDS

colorectal cancer, diffuse reflectance spectroscopy, ex vivo, in vivo, tissue classification

Train data	Test data	Compared results
Ex vivo	Ex vivo	SVM
In vivo	In vivo	SVM
Ex vivo & In vivo	Ex vivo & In vivo	SVM
Ex vivo	In vivo	SVM

## 1 | INTRODUCTION

Colorectal cancer is the third most common cancer worldwide for men and women combined and the second cause of cancer-related death [1]. Standard of care for advanced stage colorectal cancer is surgery, which is sometimes combined with neo-adjuvant chemo- and/or radiotherapy. In colorectal cancer surgery, there are two main challenges. First, complete removal of the tumor, as a positive resection margin is a negative independent predictor of survival and local recurrence [2, 3]. Second, avoiding very extensive surgery to prevent complications from

damage to vital structures. Technology for intraoperative tissue classification could be of great benefit to decrease the number of positive resection margins, while preventing complications due to very extensive surgery.

Fiberoptic diffuse reflectance spectroscopy (DRS) can be used for intraoperative tissue classification. In DRS, light over a broad wavelength range is sent through an optical fiber into the tissue. Within the tissue, the light will undergo scattering and absorption, which depends on tissue characteristics and varies with the wavelength of the light [4, 5]. Part of the light will be scattered back to the surface of the tissue where

This is an open access article under the terms of the Creative Commons Attribution License, which permits use, distribution and reproduction in any medium, provided the original work is properly cited.

© 2019 The Authors. *Translational Biophotonics* published by WILEY-VCH Verlag GmbH & Co. KGaA, Weinheim

it can be collected with a second fiber. Based on the collected spectrum, different tissue types can be distinguished [5].

DRS has been used before for tissue classification in cancers, like breast, head and neck, liver, lung and also colorectal cancer [6–12]. In colorectal cancer, most research was done during endoscopy to detect tumor tissue inside the lumen, where only mucosal tissue and tumor tissue can be encountered [13–17]. However, during surgery, tissue is assessed from outside the lumen, where no mucosal tissue but mainly fat and healthy colorectal wall are present. This makes classification during surgery different compared to the endoscopic setting. Some studies have been focused on the use of DRS during colorectal cancer surgery, with accuracies ranging from 91% to 95%. However, all these studies were performed *ex vivo* [9, 10, 12]. In order to use DRS during surgery, *in vivo* use of DRS has to be evaluated as well. Data acquisition *in vivo* during colorectal cancer surgery is more complicated and less controlled compared to the *ex vivo* setting, in terms of pressure applied on the probe, correlation with pathology and ambient light control. Therefore, it would be of great benefit if data obtained *ex vivo* could be used reliably to train a classifier intended for *in vivo* use.

So far, not many studies have focused on the question whether results obtained *ex vivo* can be used for *in vivo* application. One study on mouse ear models was done in which DRS data were obtained in living mice (*in vivo*), 5 to 10 minutes after excision (*ex vivo*) of tissue and after 24 and 72 hours of storage [18]. Furthermore, a study was done on human nerves during surgery and postmortem [19]. Both studies found differences between *in vivo* measurements and *ex vivo* measurements. However, both studies were focused on *ex vivo* measurements after long-term storage. Therefore, in the current study, *in vivo* and *ex vivo* measurements are performed on colorectal cancer specimen during surgery and within 1 hour after resection. Measurement locations were marked *in vivo* to direct the *ex vivo* measurements and to allow accurate pathology registration. A mixed-effect linear regression is done to compare the results obtained *in vivo* and *ex vivo*. Furthermore, a classifier is trained using the *ex vivo* data and tested on the *in vivo* data to examine if a similar accuracy is obtained compared to the classification trained and tested on *in vivo* data.

## 2 | MATERIALS AND METHODS

### 2.1 | Measurement setup

The DRS system used for this study consisted of two spectrometers and tungsten halogen light source with embedded shutter. One spectrometer resolves light in the visual wavelength range, 400 to 1100 nm (Andor Technology, DU420ABRDD); the other resolves light in the near-infrared wavelength range, 900 to 1700 nm (Andor Technology,


DU492A-1.7). The light source emits light from 360 to 2500 nm. The system is controlled by custom-made LabView software (National Instruments, Austin, Texas). A detailed description of the calibration of the system can be found elsewhere [20, 21].

Measurements were performed using clinical-grade disposable 16 G needles (INVIVO, Gainesville, Florida). Three optical fibers with a core diameter of 200  $\mu\text{m}$  were embedded in the needle, one to transport the light from the source to the tissue and two to transport the light from the tissue to the two spectrometers. The center-to-center distance between the delivering fiber and the two collecting fibers was 1.29 mm (Figure 1).

### 2.2 | Data acquisition

This study was performed under approval from the internal review board (Dutch Trial Register NTR5315). Patients with colorectal cancer, who had to undergo open surgery to remove the tumor, in the Netherlands Cancer Institute, were included. All patients were included based on preoperative imaging, which indicated advanced stage colorectal cancer, stage T3 or T4. All included patients signed informed consent. All ethical guidelines were followed.

The surgeon was asked to perform measurements during surgery by placing the needle on healthy fat, healthy colorectal wall and tumor. All measurement locations were marked with a suture. After resection, the measurements were repeated *ex vivo* on the marked locations. These

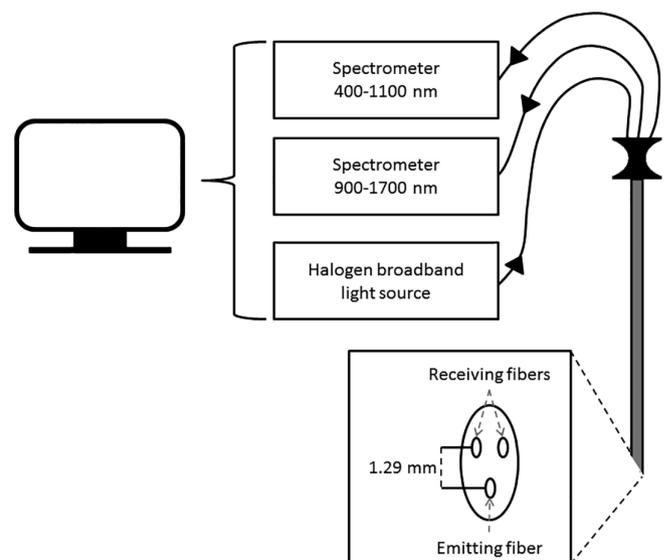

**FIGURE 1** Schematic of the measurement setup. The setup includes two spectrometers and a halogen broadband light source. The measurement needle contains three fibers, one to transport light to the tissue and two to transport the light from the tissue to the two spectrometers

measurements were performed using the same needle that was used in vivo. After the ex vivo measurements, the sutures were removed and ink was used to mark the measurement locations. Thereafter, the specimen was brought to the pathology department where the specimen was processed according to standard protocol. After fixation, pathology slides were obtained for all measured locations. These pathology slides were annotated by a pathologist to obtain a ground truth for all measured locations.

## 2.3 | Data processing

The spectra obtained from the two spectrometers were stitched together before performing a single parameter fit using an analytical model, based on optical diffusion theory, to obtain tissue constituents and optical properties of the measured tissue volume [20]. This model uses known absorption spectra and scattering characteristics of constituents present in the measured volume to fit a spectrum to the measured reflectance and generates estimations of the tissue constituents and scattering characteristics. The model has been described in detail elsewhere [4, 20]. For this study, a model with 12 parameters was used, four focused on blood, two on water and fat, three parameters were focused on scattering properties and a single parameter for collagen, beta-

carotene and a scale factor (Table 1). The scale factor couples the incident collimated light to the diffuse field in the tissue and is related to the scattering phase function [4]. The model was fitted on the measured spectra using a Levenberg-Marquardt least squares minimization method. Based on the confidence intervals obtained for all fitted parameters and based on the deviation between the measured spectrum and the obtained fit, using the relative residual, bad fits were excluded from the analysis. The relative residual was computed by dividing the absolute difference between the measured spectrum and obtained fit by the mean of the measured spectrum. If the relative residual was above 0.9, the fit was excluded. The analytical model enabled the detection of possible differences between in vivo and ex vivo to biological parameters.

## 2.4 | Statistics

A mixed-effect linear regression was performed to compare fitted parameters between in vivo data and ex vivo measurements, and between tissue-type measurements. A cross-classified data structure (Figure 2) was taken into account to model correlation between all measurements performed within one patient in the different tissue type and measurement type.


Separate regression models were fitted to compare in vivo and ex vivo measurements within each tissue type. Furthermore, comparisons between tumor and fat, and tumor and healthy colorectal wall, were performed, for the in vivo and ex vivo measurements, separately. All *P*-values of .05 or lower were considered significant.

## 2.5 | Classification

Classification of the measurements was performed using a linear support vector machine (SVM). Due to the multiclass database, three binary SVMs were used to obtain a complete classification of the dataset. The three binary classifiers included one for fat vs healthy colorectal wall, one for fat vs tumor and one for healthy colorectal wall vs tumor. The SVM was trained and tested using a leave-one-patient-

**TABLE 1** All parameters used in analytical model, grouped

Group	Parameter	Abbreviation used
Blood	Volume fraction of blood present in the tissue	Blood (%)
	Saturation of the blood	StO <sub>2</sub> (%)
	Amount of methemoglobin present	Methemoglobin
	Diameter of the blood vessels	Diameter of blood vessels
Water and fat	Volume fraction of water plus fat	Water + Fat (%)
	Volume fraction of fat from water plus fat fraction	Fat/(Water + Fat) (%)
Scattering	Scattering coefficient at 800 nm	Scattering at 800 nm
	Scattering wavelength slope	Scattering slope
	Fraction of Mie over Rayleigh scattering	Fraction of Mie scattering over Rayleigh scattering
Single parameters	Collagen	Collagen
	Beta-carotene	Beta-carotene
	Scale factor	Scale factor

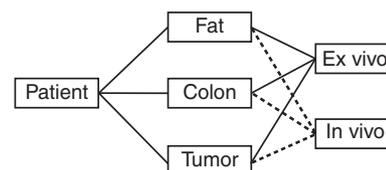

**FIGURE 2** Cross-classified data structure. A comparison between ex vivo and in vivo is made for each tissue type on a per patient basis. The lines indicate correlations between the measurements

out cross validation. Four different train and test sets were used to train and test the SVM (Table 2).

In the final classifier, the ex vivo data of the patient, of which the in vivo data were used for testing, were left out of the train dataset. All classifications were performed twice, once with all fitted parameters and once with only the selected parameters. Selection of the parameters was done using forward feature selection on only ex vivo data or on only in vivo data or on a combination of in and ex vivo data. The classifications were not optimized, but were only used to compare the difference in performance due to different train and test datasets. The performance evaluation was done using the area under the curve (AUC) of the receiver operating characteristic (ROC) curve and the Matthews correlation coefficient (MCC). The performance of the different

**TABLE 2** Overview of the four different combinations of train and test sets

Train dataset	Test dataset
Ex vivo	Ex vivo
In vivo	In vivo
Ex vivo and in vivo	Ex vivo and in vivo
Ex vivo	In vivo

**TABLE 3** Overview of all included spectra

Tissue type	In vivo	Ex vivo	Total
Fat	321	420	741
Healthy colorectal wall	172	262	434
Tumor	83	59	142
Total	576	741	1317

**TABLE 4** *P*-values of the parameters' comparison between in vivo and ex vivo for all tissue types separately

Parameter	<i>P</i> -value fat		<i>P</i> -value healthy colorectal wall		<i>P</i> -value tumor	
Blood (%)	.01	↑	.00	↑	.00	↑
StO <sub>2</sub> (%)	.00	↑	.00	↑	.00	↑
Water + Fat (%)	.00	↓	.01	↓	.03	↓
Fat/(Water + Fat) (%)	.03	↑	.05	↑	<b>.72</b>	—
Scattering at 800 nm	.00	↑	<b>.27</b>	—	<b>.58</b>	—
Scattering slope	<b>.56</b>	—	.00	↑	<b>.75</b>	—
Scale factor	<b>.30</b>	—	<b>.75</b>	—	<b>.41</b>	—
Diameter of blood vessels	<b>.96</b>	—	<b>.44</b>	—	<b>.85</b>	—
Fraction of Mie scattering over Rayleigh scattering	.05	↓	<b>.58</b>	—	.01	↑
Collagen	.01	↑	.00	↑	.00	↑
Beta-carotene	.00	↑	.00	↑	<b>.20</b>	—
Methemoglobin	.00	↓	.00	↓	.01	↓

The arrows show the direction of change from in vivo to ex vivo. The values in bold show that they are not significantly different.

classifiers was compared using the McNemar's test [22], where a *P*-value of .05 was determined as significant.

## 3 | RESULTS

### 3.1 | Inclusion

For this study, 28 patients were included, 17 male and 11 female, of 26 patients tissue was measured in vivo and ex vivo. Measurements of one patient could only be performed in vivo, because the needle could not be used anymore after the in vivo measurement. In one patient, only ex vivo measurements could be performed due to failure of the system during the in vivo measurements. The median age was 61.5 years with an interquartile range of 52.25 to 68 years. Most tumors were located in the colon ( $n = 15$ ), followed by the sigmoid ( $n = 8$ ) and the rectum ( $n = 5$ ).

In total, 1605 spectra were measured, of which 288 were excluded because a tissue type was measured which was not included in the analysis, that is, fibrosis, inflammation and necrosis ( $n = 101$ ), or because no proper fit was obtained ( $n = 187$ ). In Table 3, an overview is given of the 1317 included spectra.

### 3.2 | Statistical analysis

Table 4 shows *P*-values for the difference in parameter value between in vivo and ex vivo measurements for all parameters and each tissue type separately.

The Fat/(Water + Fat) (%), the scattering slope, the scale factor and the diameter of the blood vessels showed no significant difference between in and ex vivo in any of the tissue types. For healthy colorectal wall, the scattering at

**TABLE 5** *P*-values of the parameters' comparison between tumor and fat, and tumor and healthy colorectal wall, for in vivo and ex vivo separately

Parameter	Tumor vs fat				Tumor vs healthy colorectal wall			
	<i>P</i> -value in vivo		<i>P</i> -value ex vivo		<i>P</i> -value in vivo		<i>P</i> -value ex vivo	
Blood (%)	.09	—	.01	↓	.15	—	.34	—
StO <sub>2</sub> (%)	.00	↑	.00	↑	.00	↑	.00	↑
Water + Fat (%)	.05	↑	.47	—	.01	↑	.00	↑
Fat/(Water + Fat) (%)	.00	↑	.00	↑	.89	—	.47	—
Scattering at 800 nm	.20	—	.00	↑	.06	↓	.70	—
Scattering slope	.00	↓	.00	↓	.01	↓	.09	↑
Scale factor	.81	—	.49	—	.95	—	.20	—
Diameter of blood vessels	.09	—	.15	—	.09	—	.32	—
Fraction of Mie scattering over Rayleigh scattering	.02	↑	.33	—	.03	↑	.70	↓
Collagen	.36	—	.28	—	.71	—	.12	—
Beta-carotene	.26	—	.49	—	.10	—	.27	—
Methemoglobin	.00	↑	.08	↑	.03	↑	.18	—

The arrows show the direction of change from tumor to fat and from tumor to healthy colorectal wall.

800 nm, the scale factor, the diameter of the blood vessels and the fraction of Mie vs Rayleigh scattering had a *P*-value above .05. Finally, for tumor, the Fat/(Water + Fat) (%), scattering at 800 nm, scattering slope, scale factor, the diameter of the blood vessels and the amount of beta-carotene did not show a significant difference between in vivo and ex vivo.

Comparisons between tumor and fat, and between tumor and healthy colorectal wall for each parameter, for in vivo and ex vivo separately are shown in Table 5.

For both tumor vs fat and tumor vs healthy colorectal wall, a significant difference was seen in StO<sub>2</sub> (%) for both in vivo and ex vivo. Moreover, for tumor vs fat, a significant difference was found in the Fat/(Water + Fat) (%) and in the scattering slope, both in and ex vivo. The scattering at 800 nm was only significantly different in the ex vivo measurements for tumor vs fat. For tumor vs healthy colorectal wall, Water + Fat (%) was significantly different both in and ex vivo and the scattering slope and fraction of Mie over Rayleigh scattering were only significantly different in the in vivo measurements.

### 3.3 | Selected parameters


To obtain the most important parameters used in the classification, forward feature selection was performed three times, once on only ex vivo data, once on only in vivo data and finally on the combination of both. Based on the outcome of all three feature selections, four parameters were selected and they all were selected within the first five parameters in all three feature selections.

The four parameters included Blood (%), StO<sub>2</sub> (%), Water + Fat (%) and Fat/(Water + Fat) (%). The first three parameters all showed significant differences between in vivo and ex vivo measurements for all tissue types (Table 4). The fourth parameter did show significant difference between in and ex vivo for fat and healthy colorectal wall but not for tumor. All selected parameters were significantly different between in and ex vivo for almost all tissue types, but the difference between in and ex vivo for all tissue types was in the same direction.

Of the four selected parameters, Blood (%) only showed a significant difference between tumor and fat ex vivo (Table 5). For StO<sub>2</sub> (%), there was a significant difference between tumor and fat and tumor and healthy colorectal wall both in and ex vivo. Furthermore, the difference was in the same direction for in and ex vivo. Water + Fat (%) showed a significant difference between tumor and fat, only in vivo, and between tumor and healthy colorectal wall, both in and ex vivo. Here again, changes between in vivo and ex vivo were in the same direction. For Fat/(Water + Fat) (%), there was only a significant difference between tumor and fat, both in and ex vivo.

### 3.4 | Classification

Eight different classifiers were created, using different train and test datasets. In four out of eight classifiers, all parameters were used; for the other four classifiers, only the selected parameters were used. In Figure 3, the ROC curves obtained from all four classifiers using all parameters are shown per tissue type. As can be seen, the classification trained on ex vivo data and tested on in vivo data performed

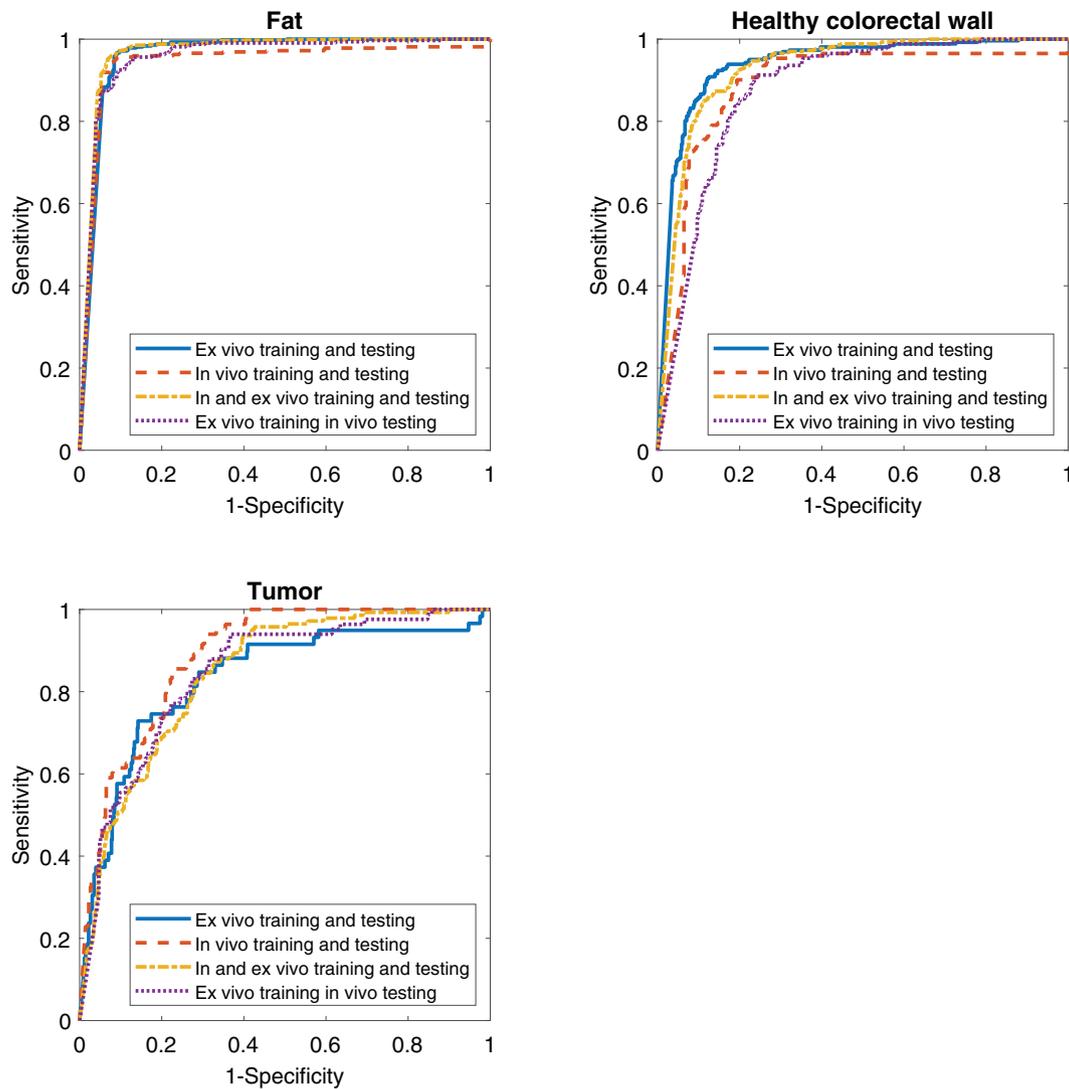

**FIGURE 3** ROC curves per tissue type of classification using different train and test datasets


**TABLE 6** AUC and MCC values for all classifier results

Tissue	Parameters	Ex vivo training and test		In vivo training and test		Ex and in vivo training and test		Ex vivo training in vivo test	
		AUC	MCC	AUC	MCC	AUC	MCC	AUC	MCC
Fat	All	0.96	0.85	0.94	0.87	0.97	0.87	0.96	0.82
	Selected	0.95	0.82	0.96	0.87	0.96	0.86	0.96	0.86
Healthy colorectal wall	All	0.94	0.76	0.89	0.63	0.93	0.73	0.88	0.62
	Selected	0.92	0.75	0.92	0.68	0.92	0.74	0.90	0.68
Tumor	All	0.83	0.33	0.89	0.41	0.84	0.33	0.84	0.48
	Selected	0.84	0.28	0.87	0.44	0.87	0.40	0.89	0.46

similar to the other classifiers, which is supported by the AUC and MCC values (Table 6). Furthermore, McNemar's test showed that there was no significant difference between the results from the classifier trained and tested on in vivo

data and the results from the classifier trained on ex vivo data and tested on in vivo data ( $P = .17$ ).

In Figure 4, the ROC curves of the classifiers using the ex vivo data as train dataset and in vivo data as test dataset are shown for all parameters and for the selected parameters.

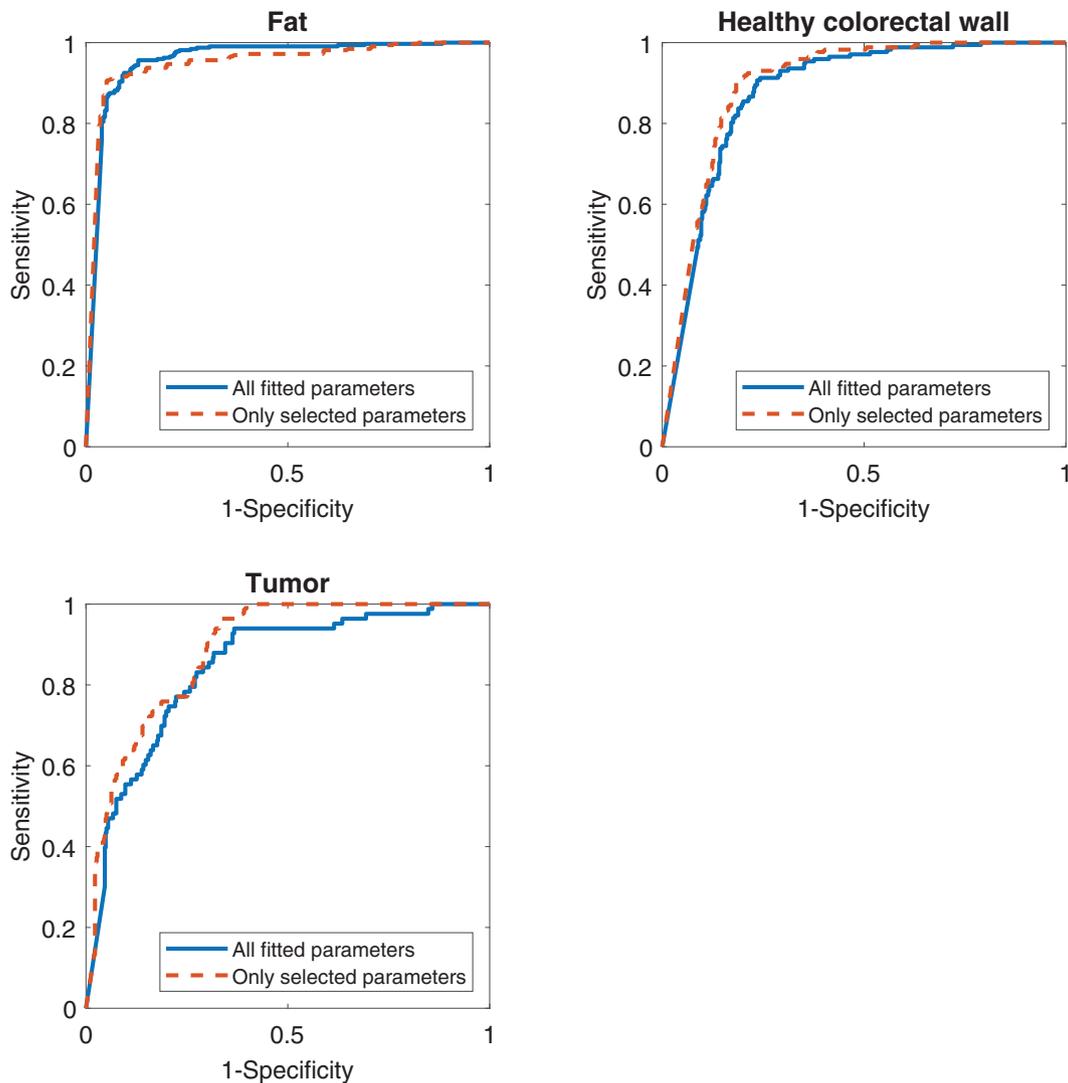

**FIGURE 4** ROC curves per tissue type, classification trained with ex vivo data and tested on in vivo data. Two classifications are performed, one with all parameters and the other with only the selected parameters

The AUC of the ROC curve for fat remained the same when only the selected parameters were used (Table 6). For healthy colorectal wall and tumor, an increase in AUC was shown when only selected parameters were used, from 0.88 to 0.90 and from 0.84 to 0.89, respectively. The MCC values of fat and healthy colorectal wall increased when only selected parameters are used, whereas the MCC value of tumor decreases.

## 4 | DISCUSSION

In this study, the potential of using ex vivo data to train a tissue classification for in vivo use is examined. AUC values of 0.96, 0.88 and 0.84 and MCC values of 0.82, 0.62 and 0.48, for fat, healthy colorectal wall and tumor, respectively, for training on ex vivo data and testing on in vivo data were

obtained. These values were comparable to the AUC and MCC values when training and testing was performed on in vivo data alone.

As a first step in this research, a statistical analysis was done on the fitted parameters to examine if there was a significant difference between in vivo and ex vivo data. Most clear difference is seen for the Water + Fat (%) and Fat/(Water + Fat) (%) parameters. A significant decrease of Water + Fat (%) was seen for all tissue types from in vivo to ex vivo. This most likely has to do with dehydration (vaporization and leakage) of the tissue when taken out of the patient. This is supported by the increase in Fat/(Water + Fat) (%) parameter for all tissue types, showing a decrease in water content. Furthermore, for all tissues, there was a significant difference in Blood (%) and StO<sub>2</sub> (%) which were both increased when measured ex vivo compared to in vivo.

Increase in Blood (%) can be explained by an increase in blood volume in the capillaries after excision [19]. The increase in StO<sub>2</sub> (%) can be explained by the exposure to air and the decrease in oxygen consumption by the cells in the specimen. These results are not in agreement with results found by Salomatina et al. [18]. In their study, comparing in and ex vivo measurements on mice ear, deoxygenation of the blood was found for the ex vivo measurements. The difference can be explained by the time between excision and measurement. In the study by Salomatina et al., the measurements were performed within 5 to 10 minutes after excision, while tissue may still be consuming oxygen, especially in the first few minutes. In our study, the time between excision and measurement was up to 1 hour. This might increase the difference in oxygenation between in vivo and ex vivo in the current study. We measured the tissues within 1 hour after resection; based on the results from previous research, results may differ when this time interval may be significantly longer.

As stated by Jacques et al., scattering parameters should be stable for a few hours after resection if overhydration and dehydration are avoided [23]. Most scattering parameters did indeed show no significant difference between in and ex vivo, except for scattering at 800 nm in fat, scattering slope in healthy colorectal wall and the fraction of Mie scattering vs Rayleigh scattering for tumor. As stated before, the decrease in Water + Fat (%) and increase in Fat/(Water + Fat) (%) most likely showed dehydration of the tissue. The changes in some scattering parameters between in vivo and ex vivo might be explained by this.

In the second step, an SVM was trained and tested on four different combinations of training and test data. When ex vivo data were used as training and in vivo data were used for testing, similar results were obtained compared to the other classifiers. This showed that using ex vivo data to create a classifier and using it afterwards to classify, in vivo data will give similar results compared to a complete in vivo study in which both training and testing of the classifier is performed on in vivo data. Using McNemar's test, no significant difference between the results of these two classifiers was found ( $P = .17$ ).

The classification results were similar if only selected parameters were used for classification. The parameters that were selected for the final classification were selected based on the results of three forward feature selections. The selected parameters did show changes between the in vivo and ex vivo setting. Parameters that are significantly different between in vivo and ex vivo might not seem useful in the classification at first. However, if these parameters either increase or decrease systematically for all tissue types, differences between tissues may still be present and they might still be of added value to the classification. For the

parameters that were not selected, any differences between tumor and fat and between tumor and healthy colorectal wall that were present ex vivo were absent or at least different for the in vivo setting.

For this study, an analytical model based on the diffusion theory was used to extract different absorption and scattering properties from the reflectance spectra of the tissue. The resulting parameters of the fit of the analytical model were used for classification instead of intensity values of the spectra as was done previously [12]. The fitted parameters were used because changes in these parameters between in vivo and ex vivo could be related to biological parameters and processes. Furthermore, because the model takes into account the fiber arrangement, results are not dependent on the measurement setup and the conclusions are therefore applicable in a more general sense. However, care should be taken that the assumptions made in the fit model are appropriate. One of the assumptions made in the diffusion theory is that the tissue is homogeneous. One can doubt whether this is an appropriate assumption for the colorectal wall which consists of several layers. However, this problem is present in the in vivo setting as well as in the ex vivo setting. Moreover, bad performance of the model due to, for instance, layered tissue will result in bad fits, which were excluded from the analysis. In this study, 11% (187 of the 1605 measurements) of the measurements were excluded based on bad performance of the fit model. So, by using the analytical model, and excluding measurements with a bad performing fit, the results obtained in this study are expected to be generalizable to other measurement setups.

## 5 | CONCLUSION

Based on the results obtained in this study, it can be concluded that at least for colorectal cancer, it is possible to train a classifier intended to classify in vivo spectra reliably using ex vivo measurements. Only parameters, that are constant between in vivo and ex vivo or change similarly over tissue types, should be used for that classification. Because ex vivo data acquisition is simpler compared to in vivo, larger databases can be used for training of a classifier that can be used in vivo. This might accelerate the development of optical techniques for surgical applications.

## ACKNOWLEDGMENTS

This work was supported by KWF-Alpe d'HuZes (NKI 2014-6596) and Philips Research, Eindhoven, The Netherlands. We are grateful for their support. This study was supported by Philips Research, Eindhoven, The Netherlands. The author who is affiliated with Philips Research (B.H.W.

H.) has financial interests in the subject matter, materials and equipment only in the sense that he is an employee of Philips. The other authors have declared that no conflict of interest exists.

## ORCID

Elisabeth J.M. Baltussen  <https://orcid.org/0000-0003-3526-8210>

## REFERENCES

- [1] F. Bray, J. Ferlay, I. Soerjomataram, R. L. Siegel, L. A. Torre, A. Jemal, *CA Cancer J. Clin.* **2018**, *68*, 394. <https://doi.org/10.3322/caac.21492>.
- [2] J. S. Park, J. W. Huh, Y. A. Park, Y. B. Cho, S. H. Yun, H. C. Kim, W. Y. Lee, H. K. Chun, *Dis. Colon Rectum.* **2014**, *57*. [http://journals.lww.com/dcrjournal/Fulltext/2014/08000/A\\_Circumferential\\_Resection\\_Margin\\_of\\_1\\_mm\\_Is\\_a.4.aspx](http://journals.lww.com/dcrjournal/Fulltext/2014/08000/A_Circumferential_Resection_Margin_of_1_mm_Is_a.4.aspx), 933.
- [3] I. D. Nagtegaal, P. Quirke, *J. Clin. Oncol.* **2008**, *26*, 303. <https://doi.org/10.1200/jco.2007.12.7027>.
- [4] T. J. Farrell, M. S. Patterson, B. Wilson, *Med. Phys.* **1992**, *19*, 879. <https://doi.org/10.1118/1.596777>.
- [5] T. M. Bydlon, R. Nachabé, N. Ramanujam, H. J. C. M. Sterenberg, B. H. W. Hendriks, *J. Biophotonics* **2015**, *8*, 9. <https://doi.org/10.1002/jbio.201300198>.
- [6] D. J. Evers, A. C. Westerkamp, J. W. Spliethoff, V. V. Pully, D. Hompes, B. H. W. Hendriks, W. Prevoo, M. L. F. van Velthuysen, R. J. Porte, T. J. M. Ruers, *Transpl. Int.* **2015**, *28*, 465. <https://doi.org/10.1111/tri.12517>.
- [7] L. L. Boer, B. G. Molenkamp, T. M. Bydlon, B. H. W. Hendriks, J. Wesseling, H. J. C. M. Sterenberg, et al., *Breast Cancer Res. Treat.* **2015**, *152*, 509. <https://doi.org/10.1007/s10549-015-3487-z>.
- [8] J. W. Spliethoff, D. J. Evers, H. M. Klomp, J. W. van Sandick, M. W. Wouters, R. Nachabe, et al., *Lung Cancer* **2013**, *80*, 165. <https://doi.org/10.1016/j.lungcan.2013.01.016>.
- [9] G. C. Langhout, J. W. Spliethoff, S. J. Schmitz, A. G. J. Aalbers, M. L. F. van Velthuysen, B. H. W. Hendriks, T. J. M. Ruers, K. F. D. Kuhlmann, *Lasers Surg. Med.* **2015**, *47*, 559. <https://doi.org/10.1002/lsm.22388>.
- [10] R. M. Schols, P. Dunias, F. P. Wieringa, L. P. S. Stassen, *Med. Eng. Phys.* **2013**, *35*, 1044.
- [11] S. G. Brouwer de Koning, B. EJM, M. B. Karakullukcu, B. Dashtbozorg, L. A. Smit, R. Dirven, et al., *J. Biomed. Opt.* **2018**, *23*, 1. <https://doi.org/10.1117/1.JBO.23.12.121611>.
- [12] E. J. M. Baltussen, P. Snæbjörnsson, S. G. Brouwer de Koning, S. HJCM, A. AGJ, N. Kok, et al., *J. Biomed. Opt.* **2017**, *22*, 106014. <https://doi.org/10.1117/1.JBO.22.10.106014>.
- [13] G. Zonios, L. T. Perelman, V. Backman, R. Manoharan, M. Fitzmaurice, J. Van Dam, et al., *Appl. Opt.* **1999**, *38*, 6628.
- [14] H.-W. Wang, J.-K. Jiang, C.-H. Lin, J.-K. Lin, G.-J. Huang, J.-S. Yu, *Opt. Express* **2009**, *17*, 2805. <https://doi.org/10.1364/OE.17.002805>.
- [15] H. K. Roy, A. Gomes, V. Turzhitsky, M. J. Goldberg, J. Rogers, S. Ruderman, K. L. Young, A. Kromine, R. E. Brand, M. Jameel, P. Vakil, N. Hasabou, V. Backman, *Gastroenterology* **2008**, *135*, 1069.
- [16] A. Dhar, K. S. Johnson, M. R. Novelli, S. G. Bown, I. J. Bigio, L. B. Lovat, S. L. Bloom, *Gastrointest. Endosc.* **2006**, *63*, 257. <https://doi.org/10.1016/J.GIE.2005.07.026>.
- [17] J. R. Mourant, I. J. Bigio, J. D. Boyer, T. M. Johnson, J. Lacey, A. G. Bohorfoush Iii, M. H. Mellow, *J. Biomed. Opt.* **1996**, *1*(2), 1–8.
- [18] E. Salomatina, A. N. Yaroslavsky, *Phys. Med. Biol.* **2008**, *53*, 2797. <https://doi.org/10.1088/0031-9155/53/11/003>.
- [19] G. C. Langhout, T. M. Bydlon, M. van der Voort, M. Müller, J. Kortsmi, G. Lucassen, et al., *Lasers Surg. Med.* **2018**, *50*, 253.
- [20] R. Nachabe, B. H. W. Hendriks, A. E. Desjardins, M. van der Voort, M. B. van der Mark, S. HJCM, *Estimation of lipid and water concentrations in scattering media with diffuse optical spectroscopy from 900 to 1600 nm* **2010**, *15*, 37010. <https://doi.org/10.1117/1.3454392>.
- [21] R. Nachabé, B. H. W. Hendriks, M. van der Voort, A. E. Desjardins, H. J. C. M. Sterenberg, *Biomed. Opt. Express.* **2010**, *1*, 1432. <https://doi.org/10.1364/BOE.1.001432>.
- [22] T. G. Dietterich, *Neural Comput.* **1998**, *10*, 1895. <https://doi.org/10.1162/089976698300017197>.
- [23] S. L. Jacques, *Phys. Med. Biol.* **2013**, *58*, R37.

**How to cite this article:** Baltussen EJM, Brouwer De Koning SG, Hendriks BHW, Józwiak K, Sterenberg HJCM, Ruers TJM. Comparing in vivo and ex vivo fiberoptic diffuse reflectance spectroscopy in colorectal cancer. *Translational Biophotonics*. 2019; 1:e201900008. <https://doi.org/10.1002/tbio.201900008>