

Final report of EURAMET.M.G-K3 regional comparison of absolute gravimeters

Falk, R.; Pálincáš, V.; Wziontek, H.; Castelein, S.; Bernard, J. D.; Rülke, A.; Greco, F.; Reudink, R.; Petrini, M.; More Authors

DOI

[10.1088/0026-1394/57/1A/07019](https://doi.org/10.1088/0026-1394/57/1A/07019)

Publication date

2020

Document Version

Final published version

Published in

Metrologia

Citation (APA)

Falk, R., Pálincáš, V., Wziontek, H., Castelein, S., Bernard, J. D., Rülke, A., Greco, F., Reudink, R., Petrini, M., & More Authors (2020). Final report of EURAMET.M.G-K3 regional comparison of absolute gravimeters. *Metrologia*, 57(1 A), 1-24. Article 07019. <https://doi.org/10.1088/0026-1394/57/1A/07019>

Important note

To cite this publication, please use the final published version (if applicable).
Please check the document version above.

Copyright

Other than for strictly personal use, it is not permitted to download, forward or distribute the text or part of it, without the consent of the author(s) and/or copyright holder(s), unless the work is under an open content license such as Creative Commons.

Takedown policy


Please contact us and provide details if you believe this document breaches copyrights.
We will remove access to the work immediately and investigate your claim.

Final Report

REGIONAL COMPARISON OF ABSOLUTE GRAVIMETERS

EURAMET.M.G-K3 Key Comparison

Pilot laboratory: Research Institute of Geodesy, Topography and Cartography, Czech Republic

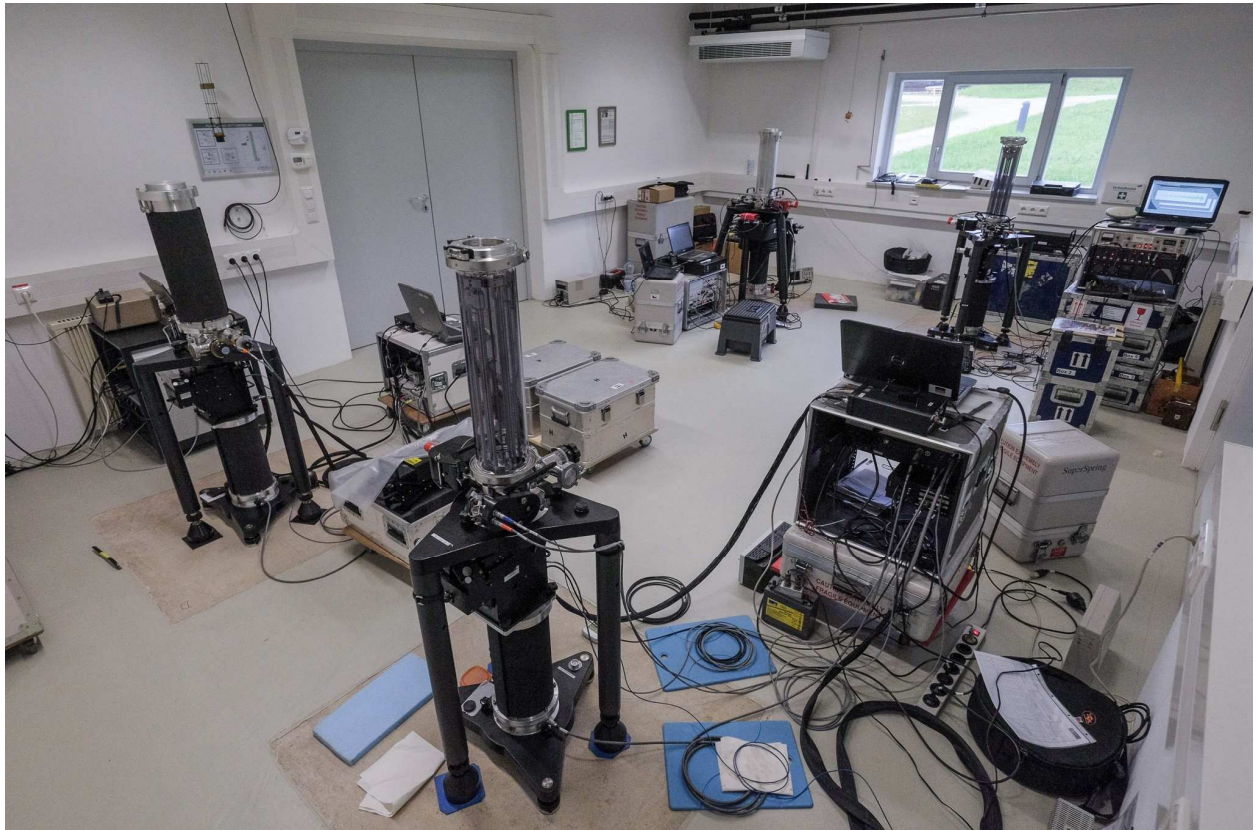

**Reinhard Falk¹, Vojtech Pálinkáš², Hartmut Wziontek¹,
Axel Rülke¹, Miloš Val'ko² and all participants**

¹ *Federal Agency of Cartography and Geodesy, Germany*

² *Research Institute of Geodesy, Topography and Cartography, Czech Republic*

Table of Content

| | |
|---|-----------|
| 1. Introduction | 3 |
| 2. List of participants | 4 |
| 3. Station description and relative gravity measurements | 5 |
| 4. Absolute gravity measurements | 6 |
| 5. Measurement strategy | 9 |
| 6. Data elaboration | 9 |
| 7. Results | 10 |
| 8. Conclusions | 15 |
| 9. References | 16 |
| Appendix A: Gravity as a function of height (vertical gravity gradients) | 17 |
| Appendix B: Additional Comparison | 18 |

1. Introduction

The Regional Key Comparison of Absolute Gravimeters, EURAMET.M.G-K3 and the simultaneously organized Additional Comparison (CCM, 2015), was held in Germany at the Geodetic Observatory Wettzell (GOW) of the German Federal Agency for Cartography and Geodesy close to the city of Bad Kötzing in the Spring of 2018. All the measurements were collected between April 16 and June 15, 2018.

The Technical Protocol (TP) was approved before the comparison by the participants and the CCM-WGG¹ (Technical protocol Version 3.0). The TP includes the list of the registered participants, a description of the comparison site, the measurement schedule and an illustrative Table to indicate the uncertainty of the gravimeters. It also specifies the data processing as well as the reporting of the results.

The schedule of absolute measurements followed the TP. However, the number of participants and their observation periods at GOW had to be changed several times, making updates of the TP necessary. Finally, 16 absolute gravimeters participated in 5 sessions.

VÚGTK/RIGTC (Research Institute of Geodesy, Topography and Cartography) under the leadership of Dr. Vojtech Pálinkáš was the Pilot Laboratory. Dr. Reinhard Falk, Dr. Axel Rülke, Dr. Hartmut Wziontek and Dr. Thomas Klügel (all of BKG) were in charge of the local organizing committee.

The EURAMET.M.G-K3 and Additional Comparison is registered as EURAMET project 1432. The comparison was organized in accordance with the CIPM MRA-D-05 of the Consultative Committee on Mass and Related Quantities (CCM). It is linked to the results of the CCM.G-K2.2017 comparison (Wu et al. 2020) in Changping (China) in 2017 by four absolute gravimeters that participated in both comparisons.

The main objective of a regional key comparison is the validation of the Calibration and Measurement Capabilities (CMCs) published in the KCDB of the BIPM through links to the CIPM KC. This is especially important for participants who could not be accommodated in the CIPM KC (CCM, 2015).

The Additional Comparison has been organized to ensure the compatibility of absolute gravimeters used for the realization of the International Gravity Reference System (Drewes and Kuglitsch 2019) and the International Database for Absolute Gravity measurements (Wziontek et al. 2012).

Here we present the list of the participants who actually performed measurements during the comparison, the data (absolute gravity measurements and their uncertainties) submitted by the operators as well as the results of the determination of the gravity as a function of height (and consequently vertical gravity gradient) at the comparison sites. The measurement strategy is briefly discussed and the results of the data harmonization is documented. Finally, the results of the adjustment are presented including the degrees of equivalence (*DoE*) of each gravimeter and the key comparison reference values (KCRV). The KCRV were obtained by the absolute values of the gravimeters participating in the KC and the gravity differences measured by all the gravimeters (including those participating at the Additional Comparison).

This report presents all results of the 5 gravimeters taking part in EURAMET.M.G-K3, the results of the Additional Comparison are documented in Annex B.

In this report, the microGal (μGal) is used as a unit of acceleration, $1 \mu\text{Gal}$ is equal to $1 \cdot 10^{-8} \text{ m/s}^2$. The standard uncertainty is denoted u ($k = 1$) and the expanded uncertainty U at a 95 % level of confidence, ($k = 2$). Sigma (σ) is denoted the standard deviation, but sometimes it also refers to standard error of estimates from least-squares adjustment, it is shown always with $k = 1$.

¹ Consultative Committee for Mass and Related Quantities - Working Group on Gravimetry
EURAMET.M.G-K3 Final Report

2. List of participants

The list of the participants is presented in Table 1. In total, 16 absolute gravimeters of three different types were compared. As to FG5 gravimeters, the FG5-202 and FG5-215 are equipped with a bulk type of interferometer. Overall, 5 teams from National Metrology Institutes (NMIs) or Designated Institutes (DIs) participated in the Key Comparison and 11 teams from non-NMI/DIs in the Additional Comparison.

Table1. Participants in the comparison (NMI = National Metrology Institute; DI = Designated Institute). The metrological institutes taking part at EURAMET.M.G-K3 are in yellow.

| Country | Institution | Gravimeter | NMI or DI | CCM.G-K2.2017 | Operator(s) |
|------------------------------|--|------------|-----------|---------------|---------------------------------------|
| EURAMET.M.G-K3 | | | | | |
| Austria | Bundesamt für Eich und Vermessungswesen (BEV), Vienna | FG5-242 | YES | YES | Christian Ullrich, Hubert Butta |
| Czech Republic | VÚGTK/ RIGTC, Geodetic Observatory Pecný | FG5-215H | YES | YES | Vojtech Pálinkáš, Jakub Kostelecký |
| Finland | Finnish Geospatial Research Institute, National Land Survey of Finland, Masala | FG5X-221 | YES | YES | Mirjam Bilker-Koivula, Jyri Näränen |
| Italy | Istituto nazionale di Ricerca Metrologica, Torino | IMGC-02 | YES | NO | Andrea Prato, Fabrizio Mazzoleni |
| Turkey | Ulusal Metroloji Enstitüsü (TUBITAK UME), Gebze-Kocaeli | FG5X-254 | YES | YES | Cafer Kirbaş, İlkan Coşkun |
| Additional Comparison | | | | | |
| Belgium | Royal Observatory of Belgium Brussels | FG5-202 | NO | NO | Michel Van Camp, Stefaan Castelein |
| France | University of Strasbourg | FG5-206 | NO | NO | Jean-Daniel Bernard |
| Germany | Federal Agency of Cartography and Geodesy (BKG) Frankfurt/Leipzig | FG5-301 | NO | YES* | Alexander Lothhammer Reinhard Falk |
| Germany | Federal Agency of Cartography and Geodesy (BKG) Frankfurt/Leipzig | FG5-101 | NO | NO | Alexander Lothhammer |
| Germany | Leibniz Universität Hannover | FG5X-220 | NO | NO | Manuel Schilling, Ludger Timmen |
| Italy | Agenzia Spaziale Italiana (ASI) / e-geos, Matera | FG5-218 | NO | NO | Domenico Iacovone, Giovanni Nettis |
| Italy | Istituto Nazionale di Geofisica e Vulcanologia (INGV) | FG5-238 | NO | NO | Filippo Greco, Alfio Alex Messina |
| Netherlands | Delft University of Technology | FG5-234 | NO | NO | René Reudink, Michele Petrini |
| Poland | Institute of Geodesy and Cartography Warszawa | A10-020 | NO | NO | Przemysław Dykowski, Marcin Sękowski |
| Slovakia | Slovak University of Technology in Bratislava | FG5X-247 | NO | NO | Juraj Janák, Juraj Papčo |
| Sweden | Lantmäteriet Gävle | FG5X-233 | NO | NO | Andreas Engfeldt, Holger Steffen |

* FG5-301 of non NMI/DI took part in the Pilot Study part of the CCM.G-K2.2017

Participants in the relative measurements

Przemysław Dykowski and Marcin Sękowski:
Institute of Geodesy and Cartography, Warszawa, Poland
and

Andreas Reinhold, Jan Müller, Reinhard Falk and Alexander Lothhammer:
Federal Agency of Cartography and Geodesy, Germany.

3. Station description and relative gravity measurements

The comparison was held in the New Gravity Laboratory at the Geodetic Observatory Wettzell (GOW) of the German Federal Agency for Cartography and Geodesy (BKG) close to the city of Bad Kötzing, situated in the Bavarian Forest in South East of Germany. The laboratory is located far from sources of anthropogenic noise (e.g. traffic). All measurements were performed on 4 separate pillars (sites) with size of 1.2 m x 1.2 m x 1.7 m (Figure 1). The site coordinates are 49.14483° North, 12.87631° East and the altitude is 606.57 m.

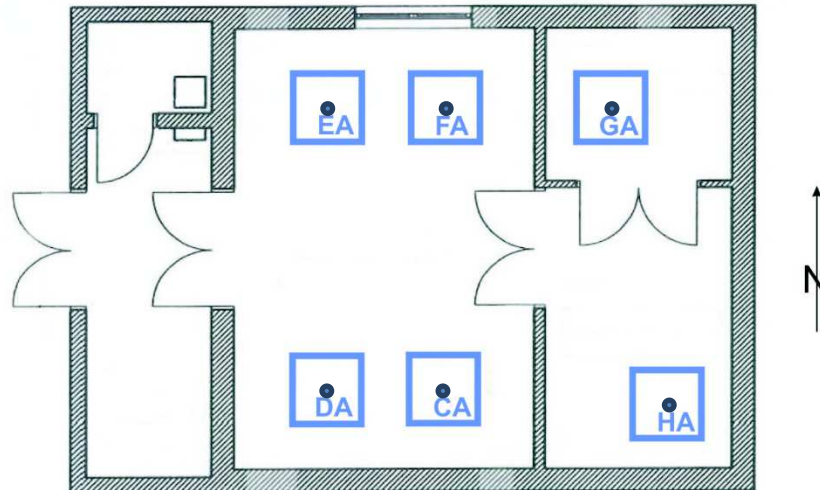


Figure 1. Sketch and Photo of the New Gravity Laboratory at Geodetic Observatory Wettzell on May 15, 2018. The pillar G is occupied by the SG030 and for AG measurements the central room is equipped with 4 pillars. The pillar H was not used during the comparison. The surface centre of each pillar is marked by a small brass benchmark, indicating the position A at each pillar.

To determine Vertical Gravity Gradients (VGGs) measurements were carried out with 3 Scintrex CG-5, 1 CG-6 and 2 LaCoste&Romberg model G gravimeters (with LRFB-300 feedback) at 2 or 3 different vertical levels at each site. The gravity as a function of height above the 4 sites were approximated by a linear function. The corresponding constant values of VGGs (derivatives of linear approximations) including standard uncertainties are shown in Table 2, results of measurements can be found in Annex A.

Table 2. Vertical gravity gradients at the 4 sites used for the comparison.

| Site | VGG / $\mu\text{Gal} \cdot \text{m}^{-1}$ | u_{VGG} / $\mu\text{Gal} \cdot \text{m}^{-1}$ |
|------|--|---|
| CA | -328.7 | 1.2 |
| DA | -330.1 | 1.1 |
| EA | -319.5 | 0.9 |
| FA | -319.9 | 0.9 |

The tidal parameters (Table 3) were estimated from 10 years of continuous measurements of the superconducting gravimeter GWR SG-029 installed at the Old Gravity Laboratory of GOW, at a distance of about 215 m from the New Gravity Laboratory.

Table 3. Simplified model of tidal parameters for Wettzell derived from 10 years of continuous observation with the superconducting gravimeter SG-029.

| Wave | Start freq. /cpd | End freq. /cpd | Amplitude factor | Phase lag /deg |
|-------|------------------|----------------|------------------|----------------|
| M0+S0 | 0.000000 | 0.000010 | 1.00000 | 0.00000 |
| SA | 0.000011 | 0.003426 | 1.16000 | 0.00000 |
| SSA | 0.004709 | 0.010952 | 1.16000 | 0.00000 |
| Mm | 0.025812 | 0.044652 | 1.16448 | -0.22820 |
| Mf | 0.060132 | 0.080797 | 1.14607 | 0.54690 |
| Mtm | 0.096423 | 0.249951 | 1.14570 | 0.40950 |
| Q1 | 0.721500 | 0.906315 | 1.14617 | -0.16000 |
| O1 | 0.921941 | 0.940487 | 1.14852 | 0.12220 |
| M1 | 0.958086 | 0.974188 | 1.15165 | 0.20040 |
| P1 | 0.989049 | 0.998028 | 1.14896 | 0.16850 |
| S1 | 0.999853 | 1.000147 | 1.12175 | 2.99680 |
| K1 | 1.001825 | 1.003651 | 1.13560 | 0.22390 |
| Psi1 | 1.005329 | 1.005623 | 1.25164 | 0.91950 |
| Phi1 | 1.007595 | 1.013689 | 1.16481 | -0.18350 |
| J1 | 1.028550 | 1.044800 | 1.15572 | 0.10940 |
| Oo1 | 1.064841 | 1.216397 | 1.15299 | 0.17630 |
| 2N2 | 1.719381 | 1.872142 | 1.16034 | 2.14020 |
| N2 | 1.888387 | 1.906462 | 1.17625 | 1.93910 |
| M2 | 1.923766 | 1.942753 | 1.18426 | 1.43640 |
| L2 | 1.958233 | 1.976926 | 1.17887 | 0.84120 |
| S2 | 1.991787 | 2.002885 | 1.18395 | 0.34170 |
| K2 | 2.004710 | 2.182843 | 1.18466 | 0.53710 |
| M3 | 2.753244 | 3.081254 | 1.06924 | 0.39180 |
| M4 | 3.791964 | 3.937897 | 0.25996 | 48.32660 |

Gravity variations during the comparison were measured with the superconducting gravimeter SG-030 at pillar G, see Figure 1. As it can be seen from Figure 2, the residual temporal gravity variations reach up to 4 μGal during the period of the comparison. These gravity variations were obtained from the measured SG signal of the lower sensor using the calibration factor of $-74.1 \mu\text{Gal/V}$ and including corrections for Earth and ocean tides (Table 3), polar motion, atmospheric effects (admittance factor of $-0.3 \mu\text{Gal/hPa}$) and an instrumental drift of $13.6 \mu\text{Gal/year}$.

4. Absolute gravity measurements

The 15 AG measurements of the 5 absolute gravimeters participating in EURAMET.M.G-K3 are listed in Table 4. Each gravimeter measured at three different sites. The reported time of the measurement is the average of the times of the observations contributing to the measurement. The submitted absolute gravity measurement g_{raw} is the mean free-fall acceleration at the individual specific measurement height which has been corrected for:

- the Earth and ocean tides, referred to the zero-tide system,
- the effect of atmospheric mass variations using the local measured air pressure record and an admittance factor of $-0.3 \mu\text{Gal/hPa}$, based on the DIN5450 (ISO 2533:1975) standard atmosphere,
- the polar motion effect, estimated from the coordinates of the Celestial Ephemeris Pole relative to the IERS Reference Pole,

- vertical gravity changes above the measurement site to obtain gravity at the specified measurement height,
- known instrumental effects (e.g. speed-of light correction, self-attraction, laser beam diffraction).

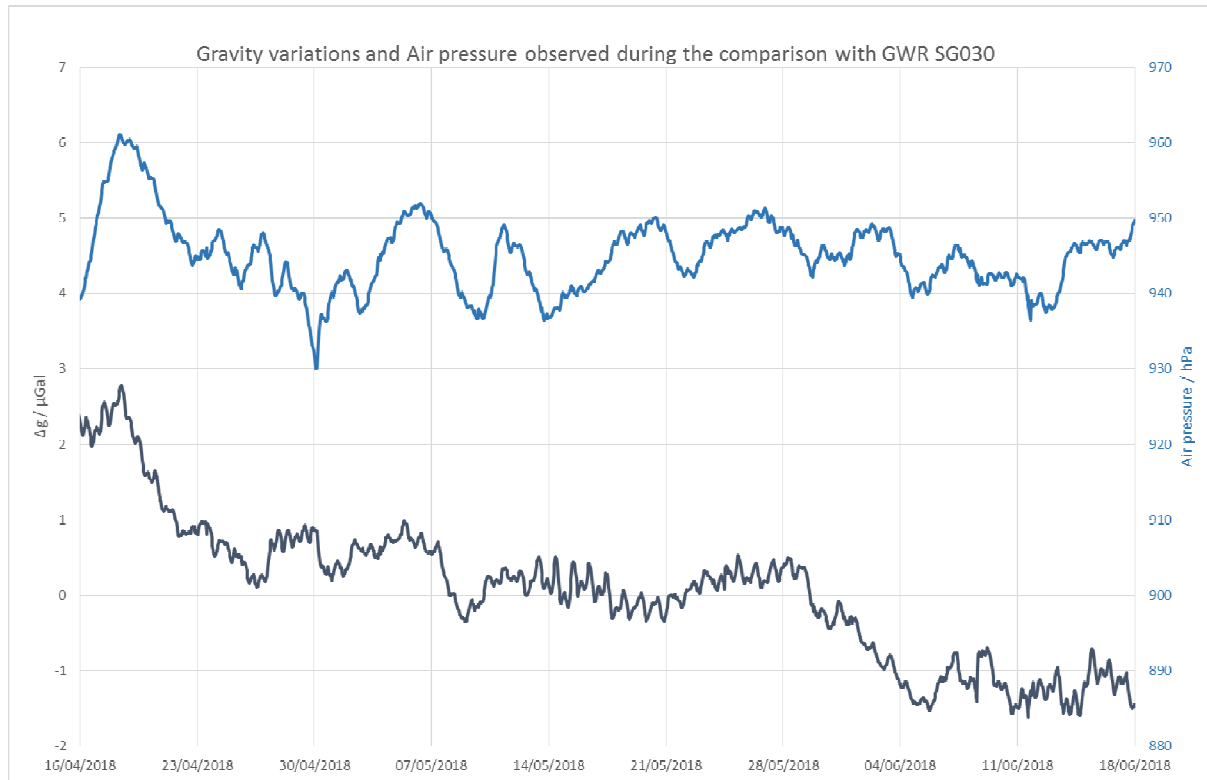


Figure 2. The residual gravity (lower graph) and air pressure (upper graph) variations observed during the comparison with the superconducting gravimeter GWR SG-030 (gravity variations in relation to the value on May 15, 2018 0:00 UT as the mean time of the comparison).

The corrections for tides, polar motion and atmospheric mass redistribution are in compliance with the International Earth Rotation and Reference Systems Service (IERS) conventions 2010 (Petit and Luzum, 2010) and IAGBN (International Absolute Gravity Base-station Network) processing standards (Boedecker, 1988).

The operators were responsible for processing their gravity data. They have submitted the final gravity values and uncertainties for all measured sites. The values g_{raw} were reported at the required measurement height using preliminary VGGs given in the TP. Due to the fact that the final VGGs (constant values for a particular site) have slightly changed, the transfer to the comparison height was performed in two steps:

1) Preliminary gradients were used for transferring reported gravity values to the instrument's reference height (distance between a benchmark and the effective position of free-fall), see Timmen (2003) and Pálinkáš et al. (2012), where the measurand is invariant of the VGG used in the equation of motion.

2) Final gradients (from Table 2) were used for transferring the values from the instrument's reference height to the comparison height of 1.250 m. The height was chosen to minimize the contribution of uncertainty from VGGs to the uncertainty of KCRV.

Residual temporal gravity variations have been taken into account by applying corrections based on the record of the superconducting gravimeter shown in Figure 2. Thus, the geophysical corrections (SGC, see Table 4) were computed as the negative value of the gravity residuals averaged over the period of the particular measurements. The uncertainty of such a correction was estimated to be 0.2 μGal .

The final values g at the comparison height of 1.250 m together with associated uncertainties u are listed in Table 4.

Table 4. List of the absolute gravity measurements during EURAMET.M.G-K3. The constant value 980,836,900.00 μGal is subtracted from all gravity values.

g_{raw} : raw gravity data with standard uncertainty u_{raw} declared by the participants, g_{raw} are corrected for all the known geophysical (tides, atmosphere, polar motion and the vertical gravity gradient) as well as instrumental effects (speed-of light correction, laser beam diffraction **DC**, self-attraction **SAC**, etc.), g_{raw} were reported at the desired measurement height **H** above the pillar using gradient **VGG₁**

dg_{ref} : gravity difference between reported height of raw gravity data and 1.250 m. * The reported measurement height slightly deviates from the usual reference instrumental height. To compute the transfer correction dg_{ref} , the default reference height of FG5 and FG5X of 1.22 m or 1.27 m, respectively was used with **VGG₁**.

g : gravity values transferred to the reference height of the comparison (125 cm) using final gradients **VGG₂** and corrected for gravity variations **SGC** based on the record of the superconducting gravimeter.

u : the standard uncertainty of g computed as root mean square of three components: the declared uncertainty of the raw gravity data by the participants u_{raw} , the transfer error to the reference height of the comparison of 1.25 m, and 0.2 μGal due to SG based corrections (SGC).

| Gravimeter | Site | Average Time | #Drops | H /cm | VGG ₁ / $\mu\text{Gal}\cdot\text{m}^{-1}$ | SAC / μGal | DC / μGal | g_{raw} / μGal | u_{raw} / μGal | VGG ₂ / $\mu\text{Gal}\cdot\text{m}^{-1}$ | dg_{ref} / μGal | SGC / μGal | g / μGal | u / μGal |
|------------|------|------------------|--------|----------|---|--------------------------|-------------------------|--------------------------------|--------------------------------|---|---------------------------------|--------------------------|--------------------------|--------------------------|
| FG5-215H | CA | 23/04/2018 23:32 | 2250 | 122.29 | -330.0 | -1.73 | 2.1 | 60.04 | 2.13 | -328.7 | -8.91 | -0.61 | 50.52 | 2.14 |
| FG5-215H | DA | 24/04/2018 21:21 | 2000 | 122.59 | -330.0 | -1.73 | 2.1 | 49.10 | 2.13 | -330.1 | -7.96 | -0.52 | 40.62 | 2.14 |
| FG5-215H | EA | 25/04/2018 20:04 | 2200 | 122.42 | -320.0 | -1.73 | 2.1 | 57.69 | 2.13 | -319.5 | -8.24 | -0.31 | 49.14 | 2.14 |
| FG5-242 | DA | 11/06/2018 23:44 | 2875 | 121.00 | -330.0 | -1.5 | 1.4 | 51.8 | 2.7 | -330.1 | -13.20 | 1.39 | 39.99 | 2.71 |
| FG5-242 | EA | 12/06/2018 18:42 | 3586 | 121.00 | -320.0 | -1.5 | 1.4 | 59.5 | 2.4 | -319.5 | -12.78 | 1.39 | 48.11 | 2.41 |
| FG5-242 | FA | 13/06/2018 22:34 | 2994 | 121.00 | -320.0 | -1.5 | 1.4 | 70.6 | 2.5 | -319.9 | -12.80 | 1.63 | 59.43 | 2.51 |
| FG5X-221 | DA | 23/04/2018 20:25 | 2148 | 126.40 | -330.0 | -1.2 | 1.4 | 38.2 | 2.3 | -330.1 | 4.62 | -0.68 | 42.14 | 2.31 |
| FG5X-221 | EA | 24/04/2018 20:08 | 2249 | 126.50 | -320.0 | -1.2 | 1.4 | 46.1 | 2.3 | -319.5 | 4.79 | -0.53 | 50.36 | 2.31 |
| FG5X-221 | FA | 25/04/2018 19:59 | 2175 | 126.50 | -320.0 | -1.2 | 1.4 | 57.3 | 2.3 | -319.9 | 4.80 | -0.31 | 61.79 | 2.31 |
| FG5X-254 | FA | 02/05/2018 18:36 | 2189 | 127.70 | -320.0 | -1.4 | 1.6 | 49.79 | 2.25 | -319.9 | 8.64 | -0.51 | 57.92 | 2.26 |
| FG5X-254 | DA | 04/05/2018 19:29 | 2098 | 127.75 | -330.0 | -1.4 | 1.6 | 30.50 | 2.23 | -330.1 | 9.08 | -0.65 | 38.93 | 2.24 |
| FG5X-254 | CA | 05/05/2018 08:34 | 598 | 127.75 | -330.0 | -1.4 | 1.6 | 43.19 | 2.38 | -328.7 | 9.04 | -0.89 | 51.34 | 2.39 |
| IMGC-02 | FA | 11/06/2018 23:08 | 471 | 47.43 | -320.0 | 0.7 | 4.43 | 299.6 | 5.0 | -319.9 | -248.15 | 1.40 | 52.85 | 5.29 |
| IMGC-02 | CA | 12/06/2018 17:51 | 537 | 47.77 | -330.0 | 0.7 | 4.43 | 310.2 | 5.0 | -328.7 | -253.86 | 1.39 | 57.73 | 5.58 |
| IMGC-02 | DA | 13/06/2018 22:35 | 553 | 47.73 | -330.0 | 0.7 | 4.43 | 294.2 | 5.0 | -330.1 | -255.07 | 1.63 | 40.76 | 5.51 |

Remark to FG5-215H: "H" is related to the modified measurement and evaluation system of the FG5-215 gravimeter that was applied also in CCM.G-K2.2017. During the comparison, the new system provided lower gravity value (by -1.7 μGal in average) than the original system. Further, following additional corrections were included into the measurements: verticality correction of +0.10 μGal , Coriolis correction of +0.50 μGal and cable length correction of -0.15 μGal .

Remark to IMGC-02: Additionally a verticality correction of +0.66 μGal was included into the measurements.

5. Measurement strategy

According to the TP, four sites were used during the comparison organized in five sessions. The first one took place from 16th to 19th of April 2018. The last session was from 11th to 16th of June 2018. Each gravimeter was planned to measure at three sites.

Table 5. Occupation of individual sites by gravimeters.

| Gravimeter | Site | | | | TOTAL |
|---|------|----|----|----|-------|
| | CA | DA | EA | FA | |
| FG5-215H | x | x | x | | 3 |
| FG5X-221 | | x | x | x | 3 |
| FG5-242 | | x | x | x | 3 |
| FG5X-254 | x | x | | x | 3 |
| IMGC-02 | x | x | | x | 3 |
| Number of KC gravimeters | 3 | 5 | 3 | 4 | |
| A10-020 | x | | x | x | 3 |
| FG5-101 | x | | x | x | 3 |
| FG5-202 | x | x | x | | 3 |
| FG5-206 | x | x | | x | 3 |
| FG5-218 | x | x | x | | 3 |
| FG5-234 | x | x | | x | 3 |
| FG5-238 | | x | x | x | 3 |
| FG5-301 | | x | x | x | 3 |
| FG5X-220 | x | | x | x | 3 |
| FG5X-233 | x | | x | x | 3 |
| FG5X-247 | x | x | | x | 3 |
| Number of gravimeters occupying each site | 12 | 12 | 11 | 13 | |

However, due to the fact that registration for the comparison was extended into the period of the comparison, the final measurement schedule could not be perfectly tuned. Thus, at least 3 KC gravimeter and at least 11 gravimeters occupied each site. The first quantity is important with respect to the definition of KCRV (in sense of absolute gravity values) and the second quantity is important to strengthen the determination of gravity differences between the KCRVs.

6. Data elaboration

A combined (observation and constraint equations) least-squares adjustment was performed using the gravity values at the reference comparison height (g) and their associated uncertainties (u) as input. Every measurement made by the gravimeter " i " (with a bias δ_i) at the site " j " during the comparison may be described by the observation equation

$$g_{ij} = g_j + \delta_i + \varepsilon_{ij} \quad (1)$$

at respective weights w_{ij} ($w_{ij} = u_o^2/u_{ij}^2$ where u_o is the unit weight).

As the set of observation equations has no unique solution for δ , a constraint, which can be interpreted as definition of the mean KCRV is required (Koo and Clare, 2012).

Generally, the consensus value of the KCRV (Koo and Clare 2012) is obtained by taking the weighted constraint,

$$\sum_{i=1}^n w_i \delta_i = d \quad (2)$$

where the w_i are the weights assigned indirect proportional to the mean uncertainty reported for each gravimeter, normalized by the condition $\sum w_i = 1$, and d is the linking converter (Jiang et al. 2013).

Due to the fact that only NMI and DI gravimeters (NMI/DIs) should contribute to the definition of KCRV, non-NMI/DI gravimeters cannot be included into the constraint nor to the determination of the linking converter d . Therefore, weights for non-NMI/DI gravimeters are all set to zero in equation (2). By this simple mathematical operation, the non-NMI/DI gravimeters are contributing only with gravity differences, according to the links between the sites.

The linking converter was computed as weighted mean of DoE determined at the CCM.G-K2.2017 (Wu et. al, 2020), see Table 6. The DoE of four linking gravimeters operated by NMI/DI have been used for this purpose.

Table 6. Determination of the linking converter as weighted mean of DoE determined at the CCM.G-K2.2017 (Wu et. al, 2020) of joint participants of the CCM.G-K2.2017 and EURAMET.M.G-K3.

| Gravimeter | DoE / μGal | $U(k=2)$ / μGal |
|---|----------------------------|-------------------------------|
| FG5-215H | -1.0 | 4.5 |
| FG5-242 | -0.1 | 6.9 |
| FG5X-221 | 0.9 | 4.7 |
| FG5X-254 | -2.7 | 4.9 |
| <i>linking converter $d =$</i> | -0.78 | 2.52 |

7. Results

7.1 The initial approach

For the initial solution of the key comparison, all the measurements presented by the operators (Table 4 and Table B1) were included in a least-squares adjustment. The reference values (RVs) and the biases (δ) are presented in Tables 7 and 8. This initial solution was computed based on Pálinkáš et.al. (2017), using the weighted constraint (Eq. 2) where the weights were computed as the normalized root mean square of the uncertainties (u) given in Table 4. Thus the values 0.292 for FG5-215H, 0.206 for FG5-242, 0.250 for FG5X-221, 0.253 for FG5X-254 are obtained. The sum of these weights is equal to 1 to ensure the correct scaling of the linking converter. The weights of the KC instrument under test (IMGC-02) and of the non NMI/DI gravimeters of the Additional Comparison (AC) have been set to zero in eq. (2).

In Pálinkáš et al. 2017 it has been shown that uncertainties of AC gravimeters should be harmonized, since their uncertainty estimates are sometimes underestimated. Such a harmonization should ensure more realistic weighting of the g -values in eq. (1). Declared uncertainties of AC FG5/X gravimeters lower than the best uncertainty declared for the KC FG5/X gravimeters ($2.13 \mu\text{Gal}$) were set to this value. In case of the A10 participating in the AC, the uncertainty was changed to $12 \mu\text{Gal}$.

No alternative solutions are presented, because, in previous reports, e.g. Pálinkáš et.al. (2017), it has been demonstrated that gravity differences determined using the non-NMI/DI meters are necessary to achieve a stable and precise solution for the CRV and that the weighted constraint represents the most appropriate way to reflect the contribution of the KC meters to the comparison reference level.

In the specific configuration of this comparison, test computations have not shown a significant difference of the variants.

Table 7. Reference Values (RVs) of the comparison using all the reported absolute measurements, reference height is 1.250 m. Results are linked by 4 instruments from NMI/DI to CCM.G-K2.2017 by means of linking converter (Table 6). The constant value 980,836,900.0 μGal is subtracted from the RVs, σ is the standard deviation of RVs from the adjustment.

| Site | RV / μGal | σ / μGal |
|------|-------------------------|-------------------------------|
| CA | 52.80 | 0.44 |
| DA | 41.34 | 0.39 |
| EA | 49.60 | 0.43 |
| FA | 59.93 | 0.43 |

Table 8. Biases δ of gravimeters at the key comparison

| Gravimeter | δ / μGal | σ / μGal |
|------------|-------------------------------|-------------------------------|
| FG5-215H | -1.15 | 0.48 |
| FG5-242 | -1.11 | 0.59 |
| FG5X-221 | 1.14 | 0.52 |
| FG5X-254 | -1.98 | 0.53 |
| IMGC-02 | -1.12 | 1.44 |

7.2 Consistency check

The consistency of measurements was checked based on the reported uncertainties. The compatibility index is defined as the ratio between the difference of the measured gravity value (g_{ij}) and the RV (g_j) at a site and its uncertainty

$$E_n = \frac{(g_{ij} - g_j)}{\sqrt{u^2(g_{ij}) + \sigma^2(g_j) + u^2(d)}} \quad (3)$$

where

- $u(g_{i,j})$... uncertainty of the g-values at the comparison height of 1.250 m,
- $\sigma(g_j)$... standard deviation of the RV at the site j obtained from the least-squares adjustment,
- u_d ... uncertainty of the linking converter.

An absolute value of E_n larger than 2 indicates that the measured gravity value is incompatible at a 95% confidence level, as the difference is not covered by the uncertainties. The compatibility index is given in Table 9.

Table 9. Consistency check: Comparison of measured gravity values g_{ij} (along with uncertainties u_{gij}) with reference values g_j (along with standard deviations $\sigma_{(g_j)}$) by means of compatibility index E_n . σ_{rep} is the short-term reproducibility of a gravimeter computed from scatter of the residuals at individual sites. The constant value 980,836,900.0 μGal has been subtracted from the gravity values.

| Gravimeter i | Site j | g_{ij} / μGal | u_{gij} / μGal | g_j / μGal | $\sigma_{(g_j)}$ / μGal | $g_{ij} - g_j$ / μGal | E_n | σ_{rep} / μGal |
|-----------------|-----------|-------------------------------|--------------------------------|----------------------------|---------------------------------------|-------------------------------------|-------|-------------------------------------|
| FG5-215H | CA | 50.52 | 2.14 | 52.80 | 0.44 | -2.28 | -0.90 | |
| FG5-215H | DA | 40.62 | 2.14 | 41.34 | 0.39 | -0.71 | -0.28 | |
| FG5-215H | EA | 49.14 | 2.14 | 49.60 | 0.43 | -0.47 | -0.18 | 0.98 |
| FG5-242 | DA | 39.99 | 2.71 | 41.34 | 0.39 | -1.35 | -0.45 | |
| FG5-242 | EA | 48.11 | 2.41 | 49.60 | 0.43 | -1.49 | -0.54 | |
| FG5-242 | FA | 59.43 | 2.51 | 59.93 | 0.43 | -0.50 | -0.17 | 0.54 |
| FG5X-221 | DA | 42.14 | 2.31 | 41.34 | 0.39 | 0.80 | 0.30 | |
| FG5X-221 | EA | 50.36 | 2.31 | 49.60 | 0.43 | 0.76 | 0.29 | |
| FG5X-221 | FA | 61.79 | 2.31 | 59.93 | 0.43 | 1.86 | 0.70 | 0.62 |
| FG5X-254 | FA | 57.92 | 2.26 | 59.93 | 0.43 | -2.01 | -0.77 | |
| FG5X-254 | DA | 38.93 | 2.24 | 41.34 | 0.39 | -2.41 | -0.93 | |
| FG5X-254 | CA | 51.34 | 2.39 | 52.80 | 0.44 | -1.46 | -0.53 | 0.48 |
| IMGC-02 | FA | 52.85 | 5.29 | 59.93 | 0.43 | -7.08 | -1.30 | |
| IMGC-02 | CA | 57.73 | 5.58 | 52.80 | 0.44 | 4.94 | 0.86 | |
| IMGC-02 | DA | 40.76 | 5.52 | 41.34 | 0.39 | -0.58 | -0.10 | 6.01 |

The compatibility index of all measurements of EURAMET.M.G-K3 is below 2, indicating consistency with the declared uncertainties. Four observations within the Additional Comparison (AC) turned out to be incompatible at the 95% confidence level (cf. Table B2), but have not been removed from the final solution, as they showed stable deviations, not affecting the gravity differences.

7.3 Final solution

Due to the fact that all measurements are consistent with the declared uncertainties, no measurements were excluded for the final solution. This means that the CRV of the initial solution (Table 7) is equivalent to the KCRV (Table 10), similarly to the *DoE* presented below which are practically equivalent with biases.

The official *DoE* (cf. Table 12 and Figure 3) were computed according to Jiang et al. (2012) using the formula

$$D_i = \left[\sum w_{ij} (g_{ij} - g_j) \right] / \sum w_{ij}. \quad (4)$$

as the weighted average difference between the measurements of a gravimeter i and the KCRV at site j . The differences between measurement and the KCRV are calculated for each gravimeter at each occupied site, see Table 11. The associated uncertainties ($U_{Di,j}$) are computed by summing up the variances of all constituents. The *DoE* are then obtained by averaging these differences (according to Eq. 4 with weights proportional to $U_{Di,j}$) and its final uncertainty (Table 12) is associated with the smallest achieved $U_{Di,j}$ (Table 11) for the particular gravimeter and labeled by U_{DoE} (Table 12).

This solution has been chosen to avoid

- 1) the *DoE* uncertainty of a gravimeter (U_{Di} in Table 11) converging towards zero with increasing numbers of measurements as discussed in Francis et al. (2015),
- 2) inconsistencies in the usual approach when *DoE* is associated with RMS of $U_{Di,j}$ that allows for associating the average *DoE* to an higher uncertainty estimate than for a single measurement of a particular gravimeter.

Table 10. Key Comparison Reference Values (KCRV) linked to the CCM.G.K-2.2017 using linking converter of $(-0.78 \pm 1.26) \mu\text{Gal}$ related to 4 NMI/DI gravimeters. The constant value 980,836,900.0 μGal was subtracted from the KCRV. U is the expanded uncertainty at 95% confidence level computed as root mean square of standard deviations σ (from the least-squares adjustment) and the uncertainty of the linking converter. The reference height is 1.250 m. The KCRV refer to May 15, 2018 0:00 UT as the mean time of the comparison.

| OFFICIAL RESULTS EURAMET.M.G-K3 KEY COMPARISON | | | |
|---|---------------------------|-------------------------------|----------------------------------|
| Site | KCRV / μGal | σ / μGal | $U (k = 2)$ / μGal |
| CA | 52.8 | 0.4 | 2.7 |
| DA | 41.3 | 0.4 | 2.6 |
| EA | 49.6 | 0.4 | 2.7 |
| FA | 59.9 | 0.4 | 2.7 |

Table 11. *DoE* of NMI/DIs determined according to Eq. 4.

g_{ij} are the measured gravity values transferred to 1.250 m with expanded uncertainty U_{ij} .

g_j are the KCRVs with associated expanded ($k = 2$) uncertainties U_j .

U_{Dij} is the expanded uncertainty of differences $g_{ij} - g_j$.

D_i is the final *DoE* computed according to Eq. 4 along with the expanded uncertainty U_{Di} (computed from U_{Dij} values, assuming statistical independence of D_{ij} values).

The constant value 980,836,900.0 μGal was subtracted from the gravity values.

| Gravimeter i | Site j | g_{ij} / μGal | U_{ij} / μGal | g_j / μGal | U_j / μGal | $D_{ij} = g_{ij} - g_j$ / μGal | U_{Dij} / μGal | D_i / μGal | U_{Di} / μGal |
|-----------------|-----------|-------------------------------|-------------------------------|----------------------------|----------------------------|--|--------------------------------|----------------------------|-------------------------------|
| FG5-215H | CA | 50.52 | 4.28 | 52.80 | 2.67 | -2.28 | 5.05 | | |
| FG5-215H | DA | 40.62 | 4.28 | 41.34 | 2.64 | -0.71 | 5.03 | | |
| FG5-215H | EA | 49.14 | 4.28 | 49.60 | 2.67 | -0.47 | 5.04 | -1.15 | 2.91 |
| FG5-242 | DA | 39.99 | 5.42 | 41.34 | 2.64 | -1.35 | 6.03 | | |
| FG5-242 | EA | 48.11 | 4.82 | 49.60 | 2.67 | -1.49 | 5.51 | | |
| FG5-242 | FA | 59.43 | 5.02 | 59.93 | 2.66 | -0.50 | 5.68 | -1.11 | 3.31 |
| FG5X-221 | DA | 42.14 | 4.62 | 41.34 | 2.64 | 0.80 | 5.32 | | |
| FG5X-221 | EA | 50.36 | 4.62 | 49.60 | 2.67 | 0.76 | 5.33 | | |
| FG5X-221 | FA | 61.79 | 4.62 | 59.93 | 2.66 | 1.86 | 5.33 | 1.14 | 3.08 |
| FG5X-254 | FA | 57.92 | 4.52 | 59.93 | 2.66 | -2.01 | 5.25 | | |
| FG5X-254 | DA | 38.93 | 4.48 | 41.34 | 2.64 | -2.41 | 5.20 | | |
| FG5X-254 | CA | 51.34 | 4.78 | 52.80 | 2.67 | -1.46 | 5.48 | -1.98 | 3.06 |
| IMGC-02 | FA | 52.85 | 10.57 | 59.93 | 2.66 | -7.08 | 10.90 | | |
| IMGC-02 | CA | 57.73 | 11.16 | 52.80 | 2.67 | 4.94 | 11.48 | | |
| IMGC-02 | DA | 40.76 | 11.03 | 41.34 | 2.64 | -0.58 | 11.34 | -1.12 | 6.49 |

The final *DoE* with uncertainty at the 95% confidence level is presented in Table 12 and Figure 3. All the gravimeters participating at EURAMET.M.G-K3 Key Comparison are in equivalence.

(*DoE* of the participating instruments of the Additional Comparison can be found in Annex B.)

Table 12. Degrees of Equivalence (DoE according to Eq. 4) of the NMI/DI gravimeters participating in the KC. The uncertainty U_{DoE} is the minimum uncertainty U_{Dij} of the 3 differences from Table 11. It represents the expanded uncertainty at 95% confidence.

| OFFICIAL RESULTS EURAMET.M.G-K3 KEY COMPARISON | | |
|---|----------------------------|--|
| Gravimeter | Degree of Equivalence | |
| | DoE / μGal | U_{DoE} ($k = 2$) / μGal |
| FG5-215H | -1.2 | 5.0 |
| FG5-242 | -1.1 | 5.5 |
| FG5X-221 | 1.1 | 5.3 |
| FG5X-254 | -2.0 | 5.2 |
| IMGC-02 | -1.1 | 10.9 |

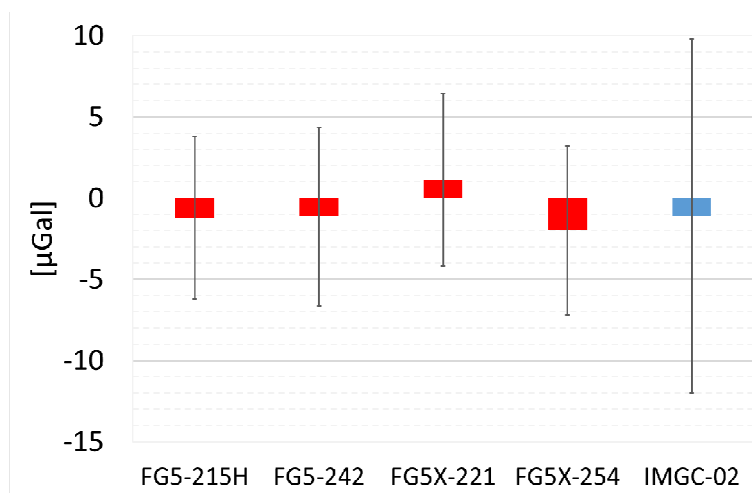


Figure 3. Degrees of Equivalence (DoE) of the NMI/DI gravimeters participating in the KC calculated from the difference between the gravimeter measurements and the KCRV for the correspondent pillar. The error bars represent the expanded uncertainties (U_{DoE}) of the DoE at 95% confidence.

8. Conclusions

Sixteen gravimeters were compared within the framework of the regional EURAMET.M.G-K3 key comparison and Additional Comparison. Five gravimeters were operated by different NMIs and DIs, these instruments participated at the EURAMET.M.G-K3 key comparison. Four of them were used to link the regional comparison to the CCM.G.K2.2017 by means of the linking converter computed as weighted average of *DoE* as documented in Wu et al. (2020) for those gravimeters.

Non-NMI/DI gravimeters participating in the Additional Comparison did not contribute to the definition of KCRV. Nevertheless, their observations were used to strengthen the determination of the gravity differences between the 4 sites.

A least-squares adjustment with a weighted constraint was used to determine the KCRV. The final *DoE* were estimated by the weighted mean of the differences between the observations at reference height and the KCRV. In case of KC gravimeters, the weights used in the adjustment and in the estimation of the *DoE* were computed from: 1) uncertainties provided by the operators, 2) the contribution of the VGG to the transfer to the comparison reference height of 1.250 m, and 3) the uncertainty of the linking converter.

In case of some AC gravimeters, the reported uncertainties were harmonized for the weighting scheme to avoid a bias in the determination of the relative ties between the sites.

In conclusion, the *DoE* of the 5 KC gravimeters are within the range of -2.0 and +1.1 μGal . For the gravimeters participating in the Additional Comparison (elaborated in Annex B), the *DoE* are between -8.9 μGal and +2.6 μGal .

All the gravimeters participating in EURAMET.M.G-K3 Key Comparison are in equivalence. By comparing Tables 6 and 12, the long-term stability of the 4 instruments participating in both key comparisons is demonstrated (Figure4).

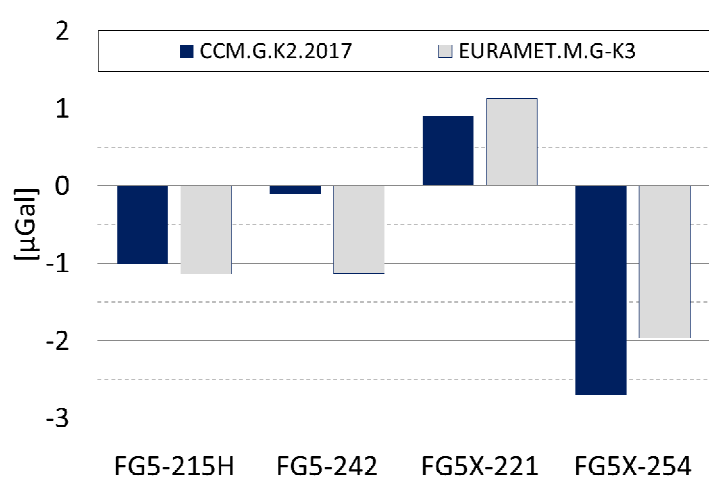


Figure 4. Joint presentation of the Degrees of equivalence of CCM.G.K2.2017 and EURAMET.M.G-K3

9. References

- Boedecker G (1988) International Absolute Gravity Base-station Network (IAGBN), Absolute Gravity Observations Data Processing Standards & Station Documentation, *BGI Bull. Inf.* **63** 51-68
- CCM (2015) CCM - IAG Strategy for Metrology in Absolute Gravimetry.
https://www.bipm.org/wg/CCM/CCM-WGG/Allowed/2015-meeting/CCM_IAG_Strategy.pdf
- Drewes H & Kuglitsch F (2019) IAG Reports 2015-2019 (Travaux de l'AIG Vol. 41), 147-149, https://iag.dgfi.tum.de/fileadmin/IAG-docs/Travaux_2015-2019.pdf
- Francis O, Baumann H, et al. (2015) CCM.G-K2 key comparison *Metrologia* **52** 07009
- Jiang Z, Pálinkáš V, Arias F E, Liard J, Merlet S, Wilmes H, Vitushkin L, et al. (2012) The 8th International Comparison of Absolute Gravimeters 2009: the first Key Comparison (CCM.G-K1) in the field of absolute gravimetry *Metrologia* **49** 666.
- Jiang Z, Pálinkáš V, Francis O, Baumann H, Makinen J, Vitushkin L, Merlet S, Tisserand L, Jousset J, Rothleitner C, Becker M, Robertsson L and Arias E F (2013) On the gravimetric contribution to watt balance experiments *Metrologia* **50** 452-471
- Koo A and Clare J F (2012) On the equivalence of generalized least-squares approaches to the evaluation of measurement comparisons *Metrologia* **49** 340-348
- Microg LaCoste : Brochure A10. (2019) <http://microglacoste.com/wp-content/uploads/2017/03/Brochure-A10.pdf> retrieved 20 September 2019.
- Pálinkáš V, Francis O, Val'ko M, Kostelecký J, Van Camp M, Castelein S, Bilker-Koivula M, Näränen J, Lothhammer A and Falk R (2017) Regional comparison of absolute gravimeters, EURAMET.M.G-K2 key comparison *Metrologia* **54** 07012
- Pálinkáš V, Jiang Z, Liard J (2012) On the effective position of the free-fall solution and the self-attraction effect of the FG5 gravimeters *Metrologia* **49** 552-559
- Petit G. and B Luzum, IERS Conventions (2010), IERS Technical Note 36, Frankfurt am Main: Verlag des Bundesamts für Kartographie und Geodäsie.
- Timmen L (2003) Precise definition of the effective measurement height of free-fall absolute gravimeters *Metrologia* **40** 62-65
- Wu S, Feng J, Li Ch et al. (2020) The results of CCM.G-K2.2017 key comparison *Metrologia* **57** 07002
- Wziontek H, Wilmes H, Bonvalot S (2012) AGrav: An International Database for Absolute Gravity Measurements. In: Kenyon S, Pacino, Marti U (eds) Geodesy for Planet Earth. International Association of Geodesy Symposia, vol 136. Springer, Berlin, Heidelberg

Annex A: Gravity as a function of height (vertical gravity gradients)

To determine Vertical Gravity Gradients (VGGs) measurements were carried out with 3 Scintrex CG-5, 1 SCINTREX CG-6 and 2 LaCoste&Romberg model G gravimeters (with LRFB-300 feedback) at 2 or 3 different vertical levels above the sites, not only during the period of the comparison, but also over the last 8 years.

All relative measurements were organized in such a way that in the upper position the sensor of the relative gravimeter was preferably positioned exactly to the reference height of 1.250 m above the marker. Such a line-up was chosen to optimize the transfer of the AG measurements to the reference height. The lower positions varied depending on the kind of instrument, used tripods and also on the specific purpose of the particular campaign.

All gravity differences measured above the same pillar are referred to the reference height of 1.250 m. The VGG was obtained from these differences by a weighted least-squares adjustment, forcing the gravity value to zero at the reference height (cf. Figure A1).

The gravity as a function of height above the 4 sites was approximated by a linear function. The corresponding constant values (VGGs as derivatives of linear functions) including standard uncertainties are shown in Table 2. Second order approximations of the gravity as a function of height could not improve the accuracy of the transfer corrections.

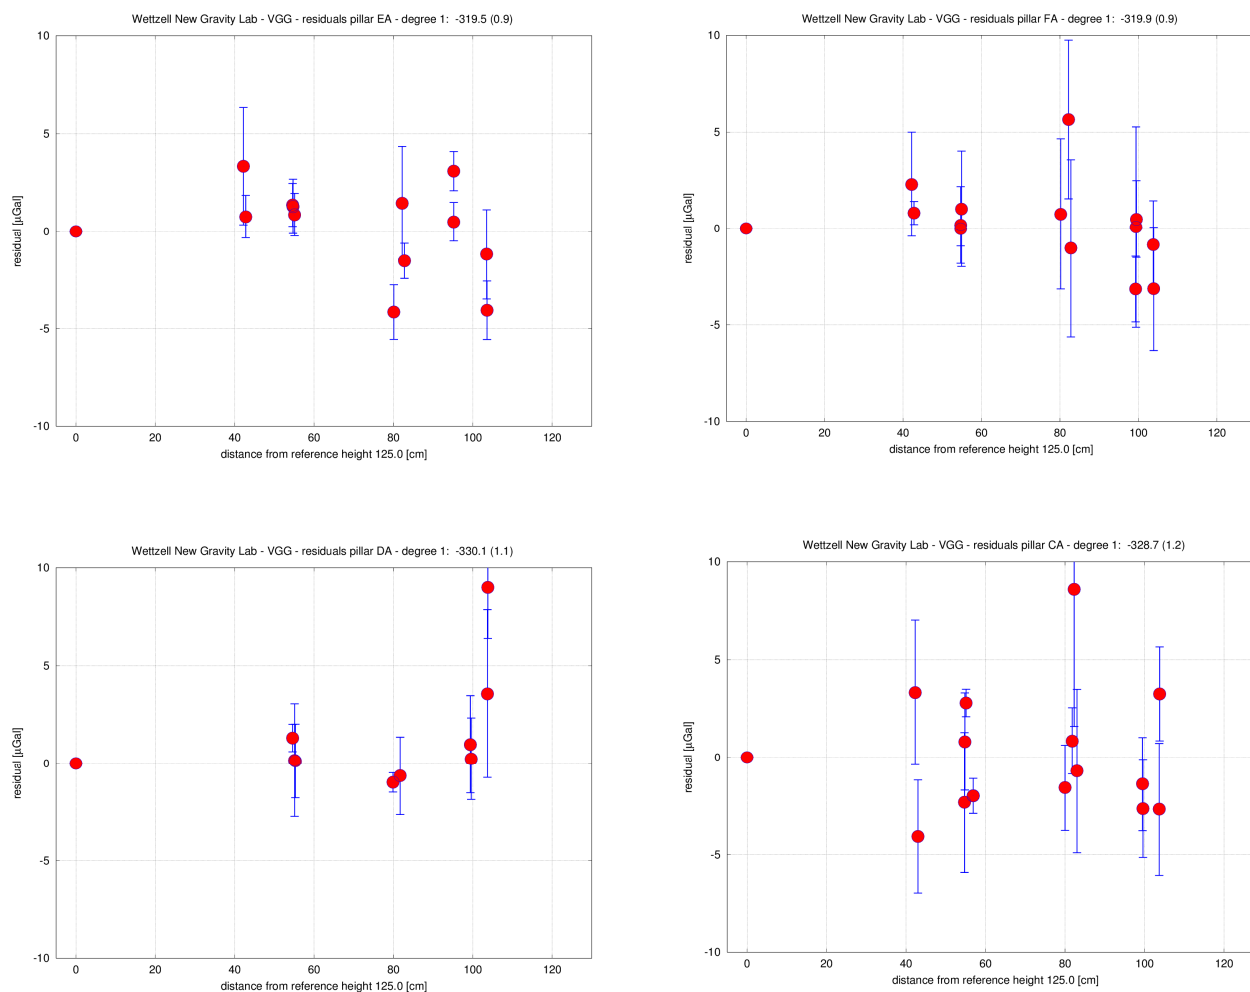


Figure A1. Results of relative gravity measurements to determine the gravity as a function of height (and consequently vertical gravity gradients) at the 4 comparison sites. Residuals of gravity differences (from measurement at the reference height of 1.250 m) are shown.

Annex B: Additional comparison

The aim of the Additional comparison was to link the European absolute gravimeters not belonging to NMI/DI to the result of the CCM.G-K2.2017 Key Comparison through the KCRV determined at EURAMET.M.G-K3 key comparison. No new adjustment has been performed. The results presented below originating from the adjustment described in section 7. KCRVs from Table 10 have been used to calculate DoE from the eq. (4).

Table B1. List of all the absolute gravity measurements (NMI/DIs are in yellow field, already shown as Table 4). The constant value 980,836,900.0 μGal is subtracted.

g_{raw} : raw gravity data with standard uncertainty u_{raw} declared by the participants, g_{raw} are corrected for all the known geophysical (tides, atmospheric pressure and polar motion effects, gravity as a function of height (here denoted as vertical gravity gradient) and instrumental effects (speed-of light correction, laser beam diffraction **DC**, self-attraction **SAC**, etc.), g_{raw} were reported at the desired measurement height **H** above the pillar using gradient **VGG₁**

dg_{ref} : gravity difference between reported height of raw gravity data and 1.250 m. * The reported measurement height slightly doesn't corresponds with the reference instrumental height. To compute the transfer correction dg_{ref} , we have used a reference height of FG5 and FG5X of 1.22 m and 1.27 m, respectively and also **VGG₁** for FG5-202, FG5-206, FG5-218 and FG5X-233.

g : gravity values transferred to the reference height of the comparison (1.250 m) using final gradients **VGG₂** and corrected for gravity variations SGC based on measurement of superconducting gravimeter.

u : the standard uncertainty of g computed as root mean square of three components: u_{raw} , the transfer error to the reference height of the comparison and 0.2 μGal due to SG based corrections (SGC).

u_{har} : harmonized standard uncertainties (see Section 7.1), computed as u but the contribution from u_{raw} of non NMI/DIs which are below 2.13 μGal were changed to 2.13 μGal . The uncertainty of the participating A10 gravimeter was harmonized to 12 μGal due to the instrument producer brochure (Microg LaCoste 2019) and the transfer to 1.250 m.

| Gravi-meter | Site | Average Time | #Drops | H /cm | VGG ₁ / $\mu\text{Gal}\cdot\text{m}^{-1}$ | SAC / μGal | DC / μGal | g_{raw} / μGal | u_{raw} / μGal | VGG ₂ / $\mu\text{Gal}\cdot\text{m}^{-1}$ | dg_{ref} / μGal | SGC / μGal | g / μGal | u / μGal | u_{har} / μGal |
|-------------|------|------------------|--------|--------|--|-----------------------|----------------------|-----------------------------|-----------------------------|--|------------------------------|-----------------------|-----------------------|-----------------------|-----------------------------|
| FG5-215H | CA | 23/04/2018 23:32 | 2250 | 122.29 | -330.0 | -1.73 | 2.1 | 60.04 | 2.13 | -328.7 | -8.91 | -0.61 | 50.52 | 2.14 | 2.14 |
| FG5-215H | DA | 24/04/2018 21:21 | 2000 | 122.59 | -330.0 | -1.73 | 2.1 | 49.10 | 2.13 | -330.1 | -7.96 | -0.52 | 40.62 | 2.14 | 2.14 |
| FG5-215H | EA | 25/04/2018 20:04 | 2200 | 122.42 | -320.0 | -1.73 | 2.1 | 57.69 | 2.13 | -319.5 | -8.24 | -0.31 | 49.14 | 2.14 | 2.14 |
| FG5-242 | DA | 11/06/2018 23:44 | 2875 | 121.00 | -330.0 | -1.5 | 1.4 | 51.8 | 2.7 | -330.1 | -13.20 | 1.39 | 39.99 | 2.71 | 2.71 |
| FG5-242 | EA | 12/06/2018 18:42 | 3586 | 121.00 | -320.0 | -1.5 | 1.4 | 59.5 | 2.4 | -319.5 | -12.78 | 1.39 | 48.11 | 2.41 | 2.41 |
| FG5-242 | FA | 13/06/2018 22:34 | 2994 | 121.00 | -320.0 | -1.5 | 1.4 | 70.6 | 2.5 | -319.9 | -12.80 | 1.63 | 59.43 | 2.51 | 2.51 |
| FG5X-221 | DA | 23/04/2018 20:25 | 2148 | 126.40 | -330.0 | -1.2 | 1.4 | 38.2 | 2.3 | -330.1 | 4.62 | -0.68 | 42.14 | 2.31 | 2.31 |
| FG5X-221 | EA | 24/04/2018 20:08 | 2249 | 126.50 | -320.0 | -1.2 | 1.4 | 46.1 | 2.3 | -319.5 | 4.79 | -0.53 | 50.36 | 2.31 | 2.31 |
| FG5X-221 | FA | 25/04/2018 19:59 | 2175 | 126.50 | -320.0 | -1.2 | 1.4 | 57.3 | 2.3 | -319.9 | 4.80 | -0.31 | 61.79 | 2.31 | 2.31 |
| FG5X-254 | FA | 02/05/2018 18:36 | 2189 | 127.70 | -320.0 | -1.4 | 1.6 | 49.79 | 2.25 | -319.9 | 8.64 | -0.51 | 57.92 | 2.26 | 2.26 |
| FG5X-254 | DA | 04/05/2018 19:29 | 2098 | 127.75 | -330.0 | -1.4 | 1.6 | 30.50 | 2.23 | -330.1 | 9.08 | -0.65 | 38.93 | 2.24 | 2.24 |
| FG5X-254 | CA | 05/05/2018 08:34 | 598 | 127.75 | -330.0 | -1.4 | 1.6 | 43.19 | 2.38 | -328.7 | 9.04 | -0.89 | 51.34 | 2.39 | 2.39 |
| IMGC-02 | FA | 11/06/2018 23:08 | 471 | 47.43 | -320.0 | 0.7 | 4.43 | 299.6 | 5.0 | -319.9 | -248.15 | 1.40 | 52.85 | 5.29 | 5.29 |
| IMGC-02 | CA | 12/06/2018 17:51 | 537 | 47.77 | -330.0 | 0.7 | 4.43 | 310.2 | 5.0 | -328.7 | -253.86 | 1.39 | 57.73 | 5.58 | 5.58 |
| IMGC-02 | DA | 13/06/2018 22:35 | 553 | 47.73 | -330.0 | 0.7 | 4.43 | 294.2 | 5.0 | -330.1 | -255.07 | 1.63 | 40.76 | 5.51 | 5.51 |

| | | | | | | | | | | | | | | | |
|----------|----|------------------|------|---------|--------|-------|------|--------|------|--------|---------|-------|-------|------|-------|
| FG5-101 | FA | 12/06/2018 23:22 | 1500 | 123.00 | -320.0 | -1.43 | 2.00 | 61.3 | 3.0 | -319.9 | -6.40 | 1.35 | 56.25 | 3.01 | 3.01 |
| FG5-101 | CA | 13/06/2018 23:10 | 1400 | 123.00 | -330.0 | -1.43 | 2.00 | 56.2 | 3.0 | -328.7 | -6.57 | 1.63 | 51.26 | 3.01 | 3.01 |
| FG5-101 | EA | 14/06/2018 20:53 | 1500 | 123.00 | -320.0 | -1.43 | 2.00 | 51.7 | 3.0 | -319.5 | -6.39 | 1.49 | 46.80 | 3.01 | 3.01 |
| FG5-202 | CA | 02/05/2018 18:17 | 2254 | 125.00* | -330.0 | -1.70 | 2.10 | 56.8 | 2.1 | -328.7 | -9.86 | -0.51 | 56.33 | 2.11 | 2.14 |
| FG5-202 | DA | 03/05/2018 19:27 | 2112 | 125.00* | -330.0 | -1.70 | 2.10 | 43.7 | 2.1 | -330.1 | -9.90 | -0.50 | 43.20 | 2.11 | 2.14 |
| FG5-202 | EA | 04/05/2018 18:17 | 2059 | 125.00* | -320.0 | -1.70 | 2.10 | 52.6 | 2.1 | -319.5 | -9.59 | -0.65 | 51.97 | 2.11 | 2.14 |
| FG5-206 | FA | 14/05/2018 22:34 | 1376 | 125.00* | -320.0 | n.a. | n.a. | 56.8 | 2.4 | -319.9 | -9.60 | 0.00 | 56.80 | 2.41 | 2.41 |
| FG5-206 | CA | 15/05/2018 13:59 | 680 | 125.00* | -330.0 | n.a. | n.a. | 48.2 | 2.4 | -328.7 | -9.86 | -0.23 | 48.01 | 2.41 | 2.41 |
| FG5-206 | DA | 16/05/2018 21:08 | 1859 | 125.00* | -330.0 | n.a. | n.a. | 36.9 | 2.4 | -330.1 | -9.90 | 0.04 | 36.94 | 2.41 | 2.41 |
| FG5-218 | CA | 14/05/2018 21:00 | 2400 | 100.00* | -330.0 | -1.36 | 1.20 | 127.71 | 2.0 | -328.7 | -9.86 | -0.04 | 45.21 | 2.01 | 2.14 |
| FG5-218 | DA | 15/05/2018 21:00 | 2400 | 100.00* | -330.0 | -1.36 | 1.20 | 119.10 | 2.0 | -330.1 | -9.90 | -0.08 | 36.52 | 2.01 | 2.14 |
| FG5-218 | EA | 16/05/2018 21:00 | 2520 | 100.00* | -320.0 | -1.36 | 1.20 | 124.16 | 2.0 | -319.5 | -9.59 | 0.02 | 44.19 | 2.01 | 2.14 |
| FG5-234 | CA | 24/04/2018 23:19 | 2600 | 121.14 | -330.0 | -1.50 | 1.00 | 65.59 | 1.90 | -328.7 | -12.69 | -0.49 | 52.41 | 1.91 | 2.14 |
| FG5-234 | DA | 25/04/2018 19:04 | 1800 | 121.27 | -330.0 | -1.50 | 1.00 | 54.05 | 1.90 | -330.1 | -12.31 | -0.18 | 41.56 | 1.91 | 2.14 |
| FG5-234 | FA | 26/04/2018 13:20 | 2100 | 121.24 | -320.0 | -1.50 | 1.00 | 71.82 | 1.89 | -319.9 | -12.03 | -0.06 | 59.73 | 1.90 | 2.14 |
| FG5-238 | DA | 14/05/2018 19:26 | 2000 | 121.60 | -330.0 | -1.50 | 1.20 | 52.1 | 3.3 | -330.1 | -11.22 | -0.02 | 40.86 | 3.31 | 3.31 |
| FG5-238 | EA | 15/05/2018 22:23 | 1800 | 122.10 | -320.0 | -1.50 | 1.20 | 59.2 | 3.2 | -319.5 | -9.27 | -0.06 | 49.87 | 3.21 | 3.21 |
| FG5-238 | FA | 16/05/2018 23:54 | 1600 | 121.50 | -320.0 | -1.50 | 1.20 | 70.9 | 3.3 | -319.9 | -11.20 | 0.06 | 59.76 | 3.31 | 3.31 |
| FG5-301 | DA | 16/04/2018 23:19 | 1300 | 122.00 | -330.0 | -1.43 | 1.10 | 53.8 | 3.1 | -330.1 | -9.90 | -2.06 | 41.84 | 3.11 | 3.11 |
| FG5-301 | EA | 17/04/2018 22:26 | 1600 | 122.00 | -320.0 | -1.43 | 1.10 | 61.7 | 3.1 | -319.5 | -9.59 | -2.32 | 49.80 | 3.11 | 3.11 |
| FG5-301 | FA | 18/04/2018 22:58 | 1600 | 122.00 | -320.0 | -1.43 | 1.10 | 73.1 | 3.1 | -319.9 | -9.60 | -2.22 | 61.28 | 3.11 | 3.11 |
| FG5X-220 | EA | 23/04/2018 22:06 | 1673 | 125.00 | -320.0 | -1.20 | 1.10 | 49.52 | 2.45 | -319.5 | 0.00 | -0.64 | 48.88 | 2.46 | 2.46 |
| FG5X-220 | FA | 24/04/2018 20:12 | 2140 | 125.00 | -320.0 | -1.20 | 1.10 | 58.33 | 2.45 | -319.9 | 0.00 | -0.53 | 57.80 | 2.46 | 2.46 |
| FG5X-220 | CA | 25/04/2018 19:58 | 1899 | 125.00 | -330.0 | -1.20 | 1.10 | 51.48 | 2.45 | -328.7 | 0.00 | -0.31 | 51.17 | 2.46 | 2.46 |
| FG5X-233 | EA | 16/04/2018 21:57 | 1200 | 120.00* | -320.0 | -1.50 | 1.00 | 62.65 | 2.4 | -319.5 | 6.39 | -2.05 | 44.59 | 2.41 | 2.41 |
| FG5X-233 | FA | 17/04/2018 19:09 | 1400 | 120.00* | -320.0 | -1.50 | 1.00 | 74.17 | 2.4 | -319.9 | 6.40 | -2.33 | 55.84 | 2.41 | 2.41 |
| FG5X-233 | CA | 18/04/2018 19:34 | 1350 | 120.00* | -330.0 | -1.50 | 1.00 | 68.48 | 2.4 | -328.7 | 6.57 | -2.35 | 49.60 | 2.41 | 2.41 |
| FG5X-247 | CA | 17/04/2018 22:04 | 3300 | 125.00 | -330.0 | n.a. | n.a. | 54.05 | 2.65 | -328.7 | 0.00 | -2.32 | 51.73 | 2.66 | 2.66 |
| FG5X-247 | DA | 18/04/2018 22:04 | 3300 | 125.00 | -330.0 | n.a. | n.a. | 42.36 | 2.00 | -330.1 | 0.00 | -2.25 | 40.11 | 2.01 | 2.14 |
| FG5X-247 | FA | 16/04/2018 22:04 | 3300 | 125.00 | -320.0 | n.a. | n.a. | 60.43 | 2.51 | -319.9 | 0.00 | -2.04 | 58.39 | 2.52 | 2.52 |
| A10-020 | CA | 16/05/2018 19:29 | 7200 | 67.83 | -330.0 | -0.60 | 1.20 | 231.6 | 4.7 | -328.7 | -187.92 | -0.01 | 43.67 | 5.05 | 12.14 |
| A10-020 | EA | 14/05/2018 19:19 | 7680 | 67.83 | -320.0 | -0.60 | 1.20 | 219.9 | 4.6 | -319.5 | -182.66 | -0.08 | 37.16 | 4.79 | 12.07 |
| A10-020 | FA | 15/05/2018 20:15 | 7680 | 67.83 | -320.0 | -0.60 | 1.20 | 237.8 | 4.7 | -319.9 | -182.89 | -0.11 | 54.80 | 4.87 | 12.07 |

Table B2. Consistency check: Comparison of measured gravity values g_{ij} (along with uncertainties u_{ij}) with reference values g_j (along with standard deviations σ_{g_j}) by means of compatibility index E_n (see eq. 3 in section 7.2). σ_{rep} is the short-term reproducibility of a gravimeter computed from scatter of the residuals at individual sites.

The constant value 980,836,900.0 μGal has been subtracted from the gravity values.

| Gravimeter i | Site j | g_{ij} / μGal | $u(g_{ij})$ / μGal | g_j / μGal | $\sigma(g_j)$ / μGal | $g_{ij} - g_j$ / μGal | E_n | σ_{rep} / μGal |
|-----------------|-----------|-------------------------------|----------------------------------|----------------------------|------------------------------------|-------------------------------------|-------|-------------------------------------|
| FG5-215H | CA | 50.52 | 2.14 | 52.80 | 0.44 | -2.28 | -0.90 | |
| FG5-215H | DA | 40.62 | 2.14 | 41.34 | 0.39 | -0.71 | -0.28 | |
| FG5-215H | EA | 49.14 | 2.14 | 49.60 | 0.43 | -0.47 | -0.18 | 0.98 |
| FG5-242 | DA | 39.99 | 2.71 | 41.34 | 0.39 | -1.35 | -0.45 | |
| FG5-242 | EA | 48.11 | 2.41 | 49.60 | 0.43 | -1.49 | -0.54 | |
| FG5-242 | FA | 59.43 | 2.51 | 59.93 | 0.43 | -0.50 | -0.17 | 0.54 |
| FG5X-221 | DA | 42.14 | 2.31 | 41.34 | 0.39 | 0.80 | 0.30 | |
| FG5X-221 | EA | 50.36 | 2.31 | 49.60 | 0.43 | 0.76 | 0.29 | |
| FG5X-221 | FA | 61.79 | 2.31 | 59.93 | 0.43 | 1.86 | 0.70 | 0.62 |
| FG5X-254 | FA | 57.92 | 2.26 | 59.93 | 0.43 | -2.01 | -0.77 | |
| FG5X-254 | DA | 38.93 | 2.24 | 41.34 | 0.39 | -2.41 | -0.93 | |
| FG5X-254 | CA | 51.34 | 2.39 | 52.80 | 0.44 | -1.46 | -0.53 | 0.48 |
| IMGC-02 | FA | 52.85 | 5.29 | 59.93 | 0.43 | -7.08 | -1.30 | |
| IMGC-02 | CA | 57.73 | 5.58 | 52.80 | 0.44 | 4.94 | 0.86 | |
| IMGC-02 | DA | 40.76 | 5.52 | 41.34 | 0.39 | -0.58 | -0.10 | 6.01 |
| FG5-101 | FA | 56.25 | 3.01 | 59.93 | 0.43 | -3.68 | -1.12 | |
| FG5-101 | CA | 51.26 | 3.01 | 52.80 | 0.44 | -1.54 | -0.47 | |
| FG5-101 | EA | 46.80 | 3.01 | 49.60 | 0.43 | -2.80 | -0.85 | 1.07 |
| FG5-202 | CA | 56.33 | 2.11 | 52.80 | 0.44 | 3.53 | 1.41 | |
| FG5-202 | DA | 43.20 | 2.11 | 41.34 | 0.39 | 1.86 | 0.75 | |
| FG5-202 | EA | 51.97 | 2.11 | 49.60 | 0.43 | 2.36 | 0.95 | 0.86 |
| FG5-206 | FA | 56.80 | 2.41 | 59.93 | 0.43 | -3.13 | -1.14 | |
| FG5-206 | CA | 48.01 | 2.41 | 52.80 | 0.44 | -4.79 | -1.74 | |
| FG5-206 | DA | 36.94 | 2.41 | 41.31 | 0.39 | -4.40 | -1.60 | 0.87 |
| FG5-218 | CA | 45.21 | 2.01 | 52.80 | 0.44 | -7.59 | -3.14 | |
| FG5-218 | DA | 36.52 | 2.01 | 41.34 | 0.39 | -4.82 | -2.00 | |
| FG5-218 | EA | 44.19 | 2.01 | 49.60 | 0.43 | -5.41 | -2.24 | 1.46 |
| FG5-234 | CA | 52.41 | 1.91 | 52.80 | 0.44 | -0.39 | -0.17 | |
| FG5-234 | DA | 41.56 | 1.91 | 41.34 | 0.39 | 0.22 | 0.09 | |
| FG5-234 | FA | 59.73 | 1.90 | 59.93 | 0.43 | -0.20 | -0.09 | 0.31 |
| FG5-238 | DA | 40.86 | 3.31 | 41.34 | 0.39 | -0.48 | -0.14 | |
| FG5-238 | EA | 49.87 | 3.21 | 49.60 | 0.43 | 0.27 | 0.08 | |
| FG5-238 | FA | 59.76 | 3.31 | 59.93 | 0.43 | -0.17 | -0.05 | 0.38 |
| FG5-301 | DA | 41.84 | 3.11 | 41.34 | 0.39 | 0.50 | 0.15 | |
| FG5-301 | EA | 49.80 | 3.11 | 49.60 | 0.43 | 0.19 | 0.06 | |
| FG5-301 | FA | 61.28 | 3.11 | 59.93 | 0.43 | 1.35 | 0.40 | 0.60 |
| FG5X-220 | EA | 48.88 | 2.46 | 49.60 | 0.43 | -0.72 | -0.26 | |
| FG5X-220 | FA | 57.80 | 2.46 | 59.93 | 0.43 | -2.13 | -0.76 | |
| FG5X-220 | CA | 51.17 | 2.46 | 52.80 | 0.44 | -1.63 | -0.58 | 0.71 |
| FG5X-233 | EA | 44.59 | 2.41 | 49.60 | 0.43 | -5.01 | -1.82 | |
| FG5X-233 | FA | 55.84 | 2.41 | 59.93 | 0.43 | -4.09 | -1.49 | |
| FG5X-233 | CA | 49.60 | 2.41 | 52.80 | 0.44 | -3.19 | -1.16 | 0.91 |
| FG5X-247 | CA | 51.73 | 2.66 | 52.80 | 0.44 | -1.07 | -0.36 | |
| FG5X-247 | DA | 40.11 | 2.01 | 41.34 | 0.39 | -1.23 | -0.51 | |
| FG5X-247 | FA | 58.39 | 2.52 | 59.93 | 0.43 | -1.54 | -0.54 | 0.24 |

| | | | | | | | | |
|---------|----|-------|------|-------|------|--------|-------|------|
| A10-020 | CA | 43.67 | 5.05 | 52.80 | 0.44 | -9.13 | -1.75 | |
| A10-020 | EA | 37.16 | 4.79 | 49.60 | 0.43 | -12.44 | -2.50 | |
| A10-020 | FA | 54.80 | 4.87 | 59.93 | 0.43 | -5.13 | -1.02 | 3.66 |

Table B3. Biases of NMI/DIs (yellow marked) and non-NMI DIs related to the approach and used weights.

| Gravimeter | δ / μGal | σ / μGal |
|------------|-------------------------------|-------------------------------|
| FG5-215H | -1.15 | 0.48 |
| FG5-242 | -1.11 | 0.59 |
| FG5X-221 | 1.14 | 0.52 |
| FG5X-254 | -1.98 | 0.53 |
| IMGC-02 | -1.12 | 1.44 |
| FG5-101 | -2.67 | 0.84 |
| FG5-202 | 2.58 | 0.64 |
| FG5-206 | -4.11 | 0.70 |
| FG5-218 | -5.94 | 0.64 |
| FG5-234 | -0.12 | 0.64 |
| FG5-238 | -0.12 | 0.90 |
| FG5-301 | 0.68 | 0.86 |
| FG5X-220 | -1.49 | 0.71 |
| FG5X-233 | -4.10 | 0.70 |
| FG5X-247 | -1.28 | 0.70 |
| A10-020 | -8.93 | 3.13 |

Table B4. *DoE* of all participating instruments determined according to Eq. 4.

g_{ij} : are the measured gravity values transferred to 1.250 m with expanded uncertainty U_{ij} .

g_j : are the KCRVs with associated expanded ($k = 2$) uncertainties U_j .

U_{Dij} : is the expanded uncertainty of differences $g_{ij}-g_j$ computed based on non harmonized uncertainties of gravimeters.

D_i : is the final *DoE* computed according to Eq. 4 along with the expanded uncertainty U_{Di} , computed from U_{Dij} values, assuming statistical independence of D_{ij} values.

The constant value 980,836,900.0 μGal was subtracted from the gravity values.

| Gravimeter i | Site j | g_{ij} / μGal | U_{ij} / μGal | g_j / μGal | U_j / μGal | $D_{ij}=g_{ij}-g_j$ / μGal | U_{Dij} / μGal | D_i / μGal | U_{Di} / μGal |
|-----------------|-----------|-------------------------------|-------------------------------|----------------------------|----------------------------|--|--------------------------------|----------------------------|-------------------------------|
| FG5-215H | CA | 50.52 | 4.28 | 52.80 | 2.67 | -2.28 | 5.05 | | |
| FG5-215H | DA | 40.62 | 4.28 | 41.34 | 2.64 | -0.71 | 5.03 | | |
| FG5-215H | EA | 49.14 | 4.28 | 49.60 | 2.67 | -0.47 | 5.04 | -1.15 | 2.91 |
| FG5-242 | DA | 39.99 | 5.42 | 41.34 | 2.64 | -1.35 | 6.03 | | |
| FG5-242 | EA | 48.11 | 4.82 | 49.60 | 2.67 | -1.49 | 5.51 | | |
| FG5-242 | FA | 59.43 | 5.02 | 59.93 | 2.66 | -0.50 | 5.68 | -1.11 | 3.31 |
| FG5X-221 | DA | 42.14 | 4.62 | 41.34 | 2.64 | 0.80 | 5.32 | | |
| FG5X-221 | EA | 50.36 | 4.62 | 49.60 | 2.67 | 0.76 | 5.33 | | |
| FG5X-221 | FA | 61.79 | 4.62 | 59.93 | 2.66 | 1.86 | 5.33 | 1.14 | 3.08 |
| FG5X-254 | FA | 57.92 | 4.52 | 59.93 | 2.66 | -2.01 | 5.25 | | |
| FG5X-254 | DA | 38.93 | 4.48 | 41.34 | 2.64 | -2.41 | 5.20 | | |
| FG5X-254 | CA | 51.34 | 4.78 | 52.80 | 2.67 | -1.46 | 5.48 | -1.98 | 3.06 |
| IMGC-02 | FA | 52.85 | 10.57 | 59.93 | 2.66 | -7.08 | 10.90 | | |
| IMGC-02 | CA | 57.73 | 11.16 | 52.80 | 2.67 | 4.94 | 11.48 | | |
| IMGC-02 | DA | 40.76 | 11.03 | 41.34 | 2.64 | -0.58 | 11.34 | -1.12 | 6.49 |

| | | | | | | | | | |
|----------|----|-------|-------|-------|------|--------|-------|-------|------|
| FG5-101 | FA | 56.25 | 6.01 | 59.93 | 2.66 | -3.68 | 6.58 | | |
| FG5-101 | CA | 51.26 | 6.01 | 52.80 | 2.67 | -1.54 | 6.58 | | |
| FG5-101 | EA | 46.80 | 6.01 | 49.60 | 2.67 | -2.80 | 6.58 | -2.67 | 3.80 |
| FG5-202 | CA | 56.33 | 4.28 | 52.80 | 2.67 | 3.53 | 5.00 | | |
| FG5-202 | DA | 43.20 | 4.28 | 41.34 | 2.64 | 1.86 | 4.98 | | |
| FG5-202 | EA | 51.97 | 4.28 | 49.60 | 2.67 | 2.36 | 4.99 | 2.58 | 2.88 |
| FG5-206 | FA | 56.80 | 4.82 | 59.93 | 2.66 | -3.13 | 5.51 | | |
| FG5-206 | CA | 48.01 | 4.82 | 52.80 | 2.67 | -4.79 | 5.51 | | |
| FG5-206 | DA | 36.94 | 4.82 | 41.34 | 2.64 | -4.40 | 5.50 | -4.11 | 3.18 |
| FG5-218 | CA | 45.21 | 4.28 | 52.80 | 2.67 | -7.59 | 4.83 | | |
| FG5-218 | DA | 36.52 | 4.28 | 41.34 | 2.64 | -4.82 | 4.81 | | |
| FG5-218 | EA | 44.19 | 4.28 | 49.60 | 2.67 | -5.41 | 4.83 | -5.94 | 2.78 |
| FG5-234 | CA | 52.41 | 4.29 | 52.80 | 2.67 | -0.39 | 4.67 | | |
| FG5-234 | DA | 41.56 | 4.28 | 41.34 | 2.64 | 0.22 | 4.65 | | |
| FG5-234 | FA | 59.73 | 4.28 | 59.96 | 2.66 | -0.20 | 4.64 | -0.12 | 2.69 |
| FG5-238 | DA | 40.86 | 6.62 | 41.34 | 2.64 | -0.48 | 7.12 | | |
| FG5-238 | EA | 49.87 | 6.41 | 49.49 | 2.67 | 0.27 | 6.95 | | |
| FG5-238 | FA | 59.76 | 6.61 | 59.93 | 2.66 | -0.17 | 7.13 | -0.12 | 4.08 |
| FG5-301 | DA | 41.84 | 6.22 | 41.34 | 2.64 | 0.50 | 6.75 | | |
| FG5-301 | EA | 49.80 | 6.21 | 49.60 | 2.67 | 0.19 | 6.76 | | |
| FG5-301 | FA | 61.28 | 6.21 | 59.93 | 2.66 | 1.35 | 6.76 | 0.68 | 3.90 |
| FG5X-220 | EA | 48.88 | 4.92 | 49.60 | 2.67 | -0.72 | 5.59 | | |
| FG5X-220 | FA | 57.80 | 4.92 | 59.93 | 2.66 | -2.13 | 5.59 | | |
| FG5X-220 | CA | 51.17 | 4.92 | 52.80 | 2.67 | -1.63 | 5.60 | -1.49 | 3.23 |
| FG5X-233 | EA | 44.59 | 4.82 | 49.60 | 2.67 | -5.01 | 5.51 | | |
| FG5X-233 | FA | 55.84 | 4.82 | 59.93 | 2.66 | -4.09 | 5.50 | | |
| FG5X-233 | CA | 49.60 | 4.82 | 52.80 | 2.67 | -3.19 | 5.51 | -4.10 | 3.18 |
| FG5X-247 | CA | 51.73 | 5.32 | 52.80 | 2.67 | -1.07 | 5.95 | | |
| FG5X-247 | DA | 40.11 | 4.28 | 41.34 | 2.64 | -1.23 | 4.81 | | |
| FG5X-247 | FA | 58.39 | 5.04 | 59.96 | 2.66 | -1.54 | 5.70 | -1.28 | 3.13 |
| A10-020 | CA | 43.67 | 10.09 | 52.80 | 2.67 | -9.13 | 10.44 | | |
| A10-020 | EA | 37.16 | 9.58 | 49.60 | 2.67 | -12.44 | 9.94 | | |
| A10-020 | FA | 54.80 | 9.74 | 59.93 | 2.66 | -5.13 | 10.10 | -8.93 | 5.86 |

All KC measurements reaching compatibility index below 2.0, therefore they are consistent with declared uncertainties. All measurements of FG5-218 and also one of A10-20 in the Additional Comparison showed to be inconsistent with declared uncertainties due to the larger bias of these gravimeters at all the measured sites. Since these gravimeters are not contributing directly to the definition of the reference, uncertainties were harmonized (for determination of KCRVs) and also due to the fact that they show short-term reproducibility of 1.5 μGal and 3.7 μGal respectively, we kept these measurements for determination of gravity differences.

The consistency of *DoE* along with declared uncertainties can be seen in Table B5. Inconsistency has been detected for the FG5-218 gravimeter.

Table B5. Degrees of Equivalence (DoE according to Eq. 5) of all gravimeters participating in the KC (yellow) and Additional Comparison. The uncertainty U_{DoE} is the minimum uncertainty U_{Dij} of the 3 differences from Table B4. It represents the expanded uncertainty at 95% confidence, computed based on declared uncertainties of participating gravimeters.

| RESULTS | | |
|--------------------------------------|----------------------------|--------------------------------|
| EURAMET.M.G-K3 KEY COMPARISON | | |
| AND ADDITIONAL COMPARISON | | |
| Gravimeter | Degree of Equivalence | |
| | DoE / μGal | U_{DoE} / μGal |
| FG5-215H | -1.2 | 5.0 |
| FG5-242 | -1.1 | 5.5 |
| FG5X-221 | 1.1 | 5.3 |
| FG5X-254 | -2.0 | 5.2 |
| IMGC-02 | -1.1 | 10.9 |
| FG5-101 | -2.7 | 6.6 |
| FG5-202 | 2.6 | 5.0 |
| FG5-206 | -4.1 | 5.5 |
| FG5-218 | -5.9 | 4.8 |
| FG5-234 | -0.1 | 4.6 |
| FG5-238 | -0.1 | 7.0 |
| FG5-301 | 0.7 | 6.8 |
| FG5X-220 | -1.5 | 5.6 |
| FG5X-233 | -4.1 | 5.5 |
| FG5X-247 | -1.3 | 4.8 |
| A10-020 | -8.9 | 9.9 |

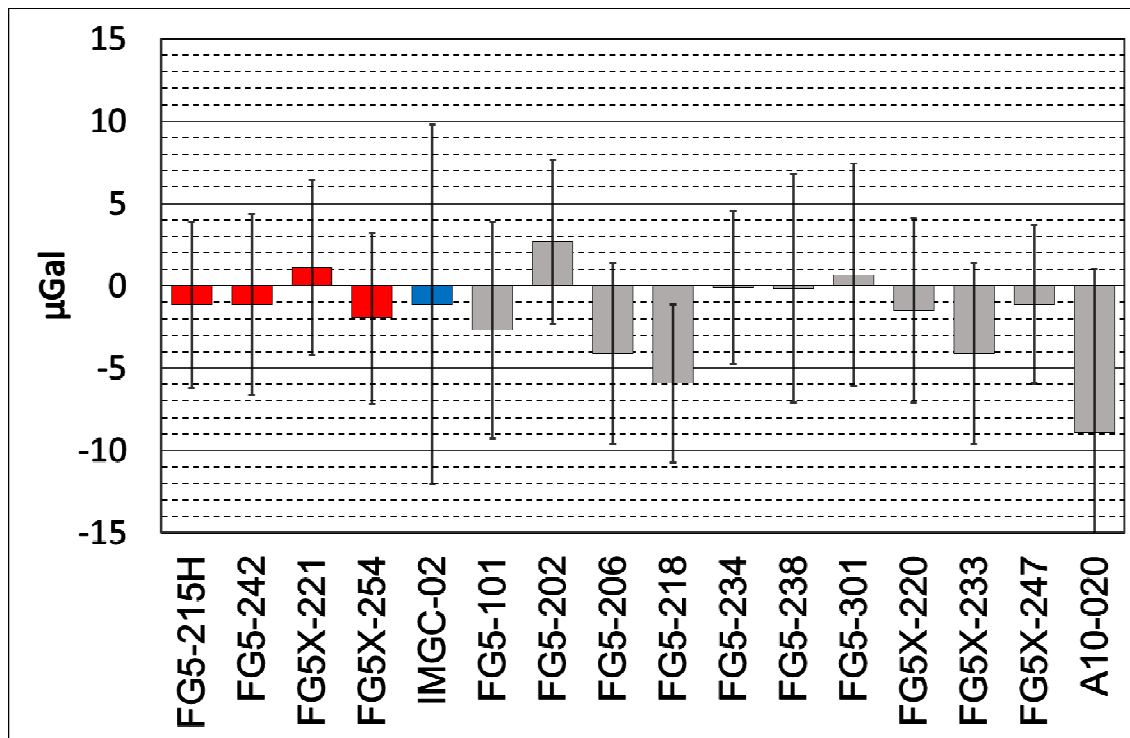


Figure B1. Degrees of equivalence of the gravimeters (linked to the CCM.G-K2.2017). The values for gravimeters of NMI/DIs are highlighted in red (participant of CCM.G-K2.2017) or blue. The error bars represent their expanded uncertainties (U_{DoE} with $k = 2$ in Table B5).

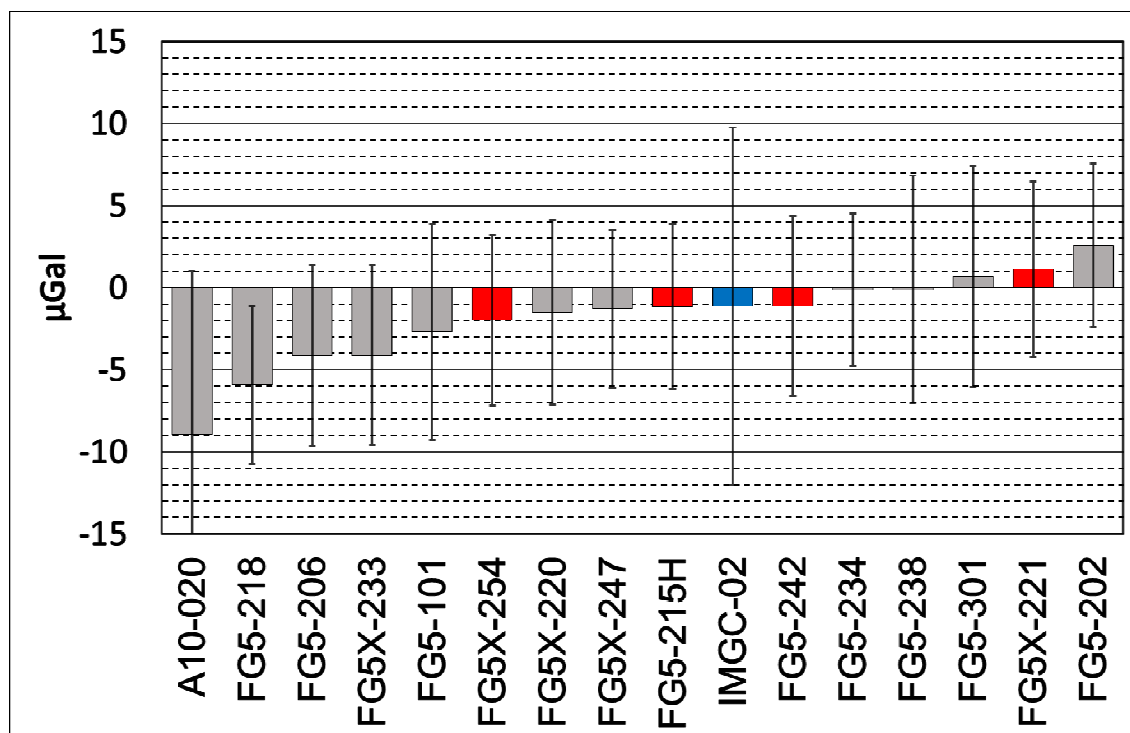


Figure B2. Degrees of equivalence of the gravimeters (linked to the CCM.G-K2.2017). The values for gravimeters of NMI/DIs are highlighted in red (participant of CCM.G-K2.2017) or blue. The error bars represent their expanded uncertainties (U_{DoE} with $k = 2$ in Table B5). The gravimeters have been rearranged according to the size of the deviation.