

Transparent Electroactive Actuators for Organ-on-Chip Platforms

Tajeddin, A.; Hunt, A.; Sarro, Pasqualina M; Mastrangeli, Massimo

Publication date
2024

Document Version
Accepted author manuscript

Citation (APA)
Tajeddin, A., Hunt, A., Sarro, P. M., & Mastrangeli, M. (2024). *Transparent Electroactive Actuators for Organ-on-Chip Platforms*. Abstract from EUROoCS Annual Meeting 2024, Milan, Italy.

Important note
To cite this publication, please use the final published version (if applicable).
Please check the document version above.

Copyright
Other than for strictly personal use, it is not permitted to download, forward or distribute the text or part of it, without the consent of the author(s) and/or copyright holder(s), unless the work is under an open content license such as Creative Commons.

Takedown policy
Please contact us and provide details if you believe this document breaches copyrights.
We will remove access to the work immediately and investigate your claim.

Alireza Tajeddin^{*1}, Andres Hunt², Pasqualina M. Sarro¹, Massimo Mastrangeli¹

1- ECTM, Department of Microelectronics, Faculty of Electrical Engineering, Mathematics and Computer Science, Delft University of Technology, Delft, The Netherlands

2- MNE, Department of Precision Microsystems Engineering, Faculty of Mechanical Engineering, Delft University of Technology, Delft, The Netherlands

*E-mail: A.Tajeddin@tudelft.nl

Micro-physiological systems (MPS) hold the potential for advancing drug research by emulating realistic *in vitro* human (patho)physiology models. These systems replicate organ microenvironments, delivering stimuli similar to those experienced by organs *in vivo*. Active biomechanical cues, like shear force and tensile stress, profoundly influence cell activity and can alter biochemical responses. The critical factors encompass the nature, duration, magnitude, and frequency of these cues [1]. A currently popular solution to provide biomechanical stimulation employs pneumatic actuation, which is powerful and multifunctional, but bulky, expensive, and inconvenient to use. Electroactive polymers (EAP), also known as artificial muscles, are gaining attention as a potential alternative for improved versatility [2]. Ionic polymer-metal composites (IPMCs) are a class of ionic EAPs which operate at low voltage and exhibit large displacement [3]. They are intrinsically suitable for cell culture media as their operating principle is based on electrolytes (Fig. 1A). However, IPMCs employ metallic electrodes, which eliminate the optical transparency essential in fundamental biological experiments.

In this study, we present the design, fabrication, and characterization of a selectively transparent IPMC for utilization in MPS to apply controllable mechanical stimuli to tissues. A multiphysics-based finite-element model was constructed and validated basing on literature data [4] to estimate the maximum tip displacement of IPMC cantilevers. The model was used to study several cantilever configurations to determine the best electrode patterning topology for the transparency, stiffness, and tip displacement trade-off. The optimized designs were implemented in wafer-scale cleanroom-compatible fabrication (Fig. 1B-C). The novel fabrication process involved sequential patterning of planar Au electrodes on polydimethylsiloxane (PDMS) substrates, and covalent bonding of a pair of such Au-patterned PDMS substrates to an ionomer (Nafion) through silanization (Fig 1B). Preliminary electro-mechanical characterization of the performance of the selectively transparent IPMC cantilevers (Fig. 1D) and biocompatibility tests indicate a potential for integration and use in MPS and organ-on-chip platforms.

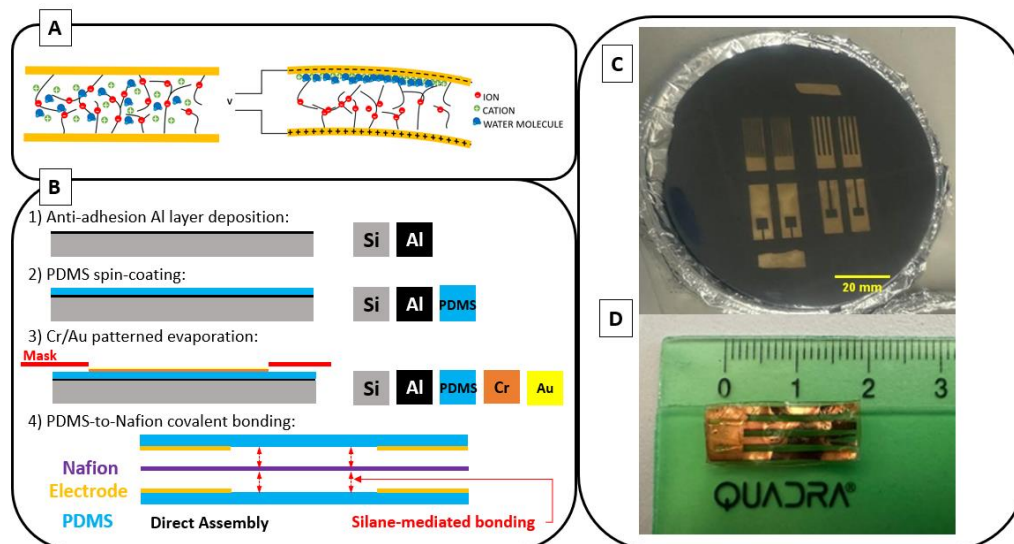


Figure 1. A) Schematic of IPMC electro-mechanical transduction mechanism. B) Fabrication steps. C) Electrodes patterned on PDMS-coated 4-inch Si wafer by shadow masking of Cr/Au e-beam evaporation. D) Released IPMC actuator.

Acknowledgments

The authors would like to thank the staff at the Else Kooi Laboratory of TU Delft for their support. This work was funded by the Netherlands Organ on-Chip Initiative (NOCI), an NWO gravitation project funded by the Ministry of Education, Culture, and Science of the government of the Netherlands (024.003.001).

References

- [1] A. W. Holle *et al.*, *Nano Lett.*, vol. 18, no. 1, pp. 1–8, Jan. 2018
- [2] M. Mastrangeli *et al.*, *21st International Conference on Solid-State Sensors, Actuators and Microsystems (Transducers)*, 2021, pp. 102–107
- [3] G. Gu *et al.*, *Frontiers in Robotics and AI*, vol. 6, p. 129, 2019
- [4] J. H. Jeon, S. W. Yeom, and I. K. Oh, *Compos Part A Appl Sci Manuf*, vol. 39, no. 4, pp. 588–596, Apr. 2008