

Feasibility of High Frame Rate 3-D Intracardiac Echography using Fan-Beam Transmissions

Soozande, Mehdi; Ossenkoppele, B.W.; Hopf, Y.M.; Pertijs, M.A.P.; Verweij, M.D.; Vos, H.J.; Bosch, J.G.; de Jong, N.

Publication date

2019

Document Version

Final published version

Citation (APA)

Soozande, M., Ossenkoppele, B. W., Hopf, Y. M., Pertijs, M. A. P., Verweij, M. D., Vos, H. J., Bosch, J. G., & de Jong, N. (2019). *Feasibility of High Frame Rate 3-D Intracardiac Echography using Fan-Beam Transmissions*. Poster session presented at 2019 IEEE International Ultrasonics Symposium, IUS 2019, Glasgow, United Kingdom.

Important note

To cite this publication, please use the final published version (if applicable).
Please check the document version above.

Copyright

Other than for strictly personal use, it is not permitted to download, forward or distribute the text or part of it, without the consent of the author(s) and/or copyright holder(s), unless the work is under an open content license such as Creative Commons.

Takedown policy

Please contact us and provide details if you believe this document breaches copyrights.
We will remove access to the work immediately and investigate your claim.

Feasibility of High Frame Rate 3-D Intracardiac Echography using Fan-Beam Transmissions

Soozande, M.; Ossenkoppele, B.W.; Hopf, Y.M.; Pertijs, M.A.P.; Verweij, M.D.; Vos, H.J.; Bosch, J.G.; de Jong, N.

Publication date

2019

Document Version

Accepted author manuscript

Published in

2019 IEEE International Ultrasonics Symposium (IUS)

Citation (APA)

Soozande, M., Ossenkoppele, B. W., Hopf, Y. M., Pertijs, M. A. P., Verweij, M. D., Vos, H. J., Bosch, J. G., & de Jong, N. (2019). Feasibility of High Frame Rate 3-D Intracardiac Echography using Fan-Beam Transmissions. In *2019 IEEE International Ultrasonics Symposium (IUS)*

Important note

To cite this publication, please use the final published version (if applicable).
Please check the document version above.

Copyright

Other than for strictly personal use, it is not permitted to download, forward or distribute the text or part of it, without the consent of the author(s) and/or copyright holder(s), unless the work is under an open content license such as Creative Commons.

Takedown policy

Please contact us and provide details if you believe this document breaches copyrights.
We will remove access to the work immediately and investigate your claim.

Feasibility of High Frame Rate 3-D Intracardiac Echography using Fan-Beam Transmissions

Mehdi Soozande¹, Boudewine Ossenkoppele², Yannick Hopf³, Michiel A.P. Pertijs³, Martin D. Verweij^{1, 2}, Hendrik J. Vos^{1, 2}, Johan G. Bosch¹, Nico de Jong^{1, 2}

¹Biomedical Engineering, Thorax Center, Erasmus MC, Rotterdam, Netherlands.

²Laboratory of Acoustical Wavefield Imaging, Department of Imaging Physics, Delft University of Technology, Delft, Netherlands.

³Electronic Instrumentation Laboratory, Delft University of Technology, Delft, Netherlands

Background, Motivation and Objective

Intracardiac echography (ICE) is widely exploited for RF ablation procedures to guide the electrophysiologist in navigating the ablation catheter. High frame rate (HFR) 3D ICE could provide 3D imaging of electromechanical wave propagation (EWI) with higher spatiotemporal resolution than conventional methods. Yet, 3D probes generally make trade-offs among channel count, image quality, and frame rate. In this work, we propose a 1D micro beamforming (MBF) approach in elevation (El) direction to reduce the channel count while maintaining a HFR and image quality comparable to a fully sampled acquisition (FSA).

Statement of Contribution/Methods

MBF is a well-established method to reduce the channel count while preserving the image quality and SNR for volumetric imaging. Generally, to suppress grating lobes and clutter, many narrow steered beams are transmitted. To achieve HFR for 3-D EWI ($>1000\text{Hz}$), the number of transmissions should be kept below 7 per volume. We propose a 1D MBF with narrow beams in El and a diverging wave in azimuth (Az) direction. We transmit a beam profile of $90^\circ \times 25^\circ$, steered from -30° to 30° , in steps of 10° . Transducer aperture is $12.5 \times 3\text{mm}$ (Az $\times$ El), consisting of 100×24 square elements, with a pitch of $125\mu\text{m}$ (7.5MHz). The final 3D image is formed by angle-weighted averaging of the sub-volumes reconstructed by voxel-based delay and sum per transmission. Image quality for different MBF sizes is compared to FSA based on lateral resolution, side-lobe levels, and contrast to noise ratio (CNR) in FIELD II simulations.

Results/Discussion

The combination of diverging wave in Az and narrow beam in El with MBF size of 3-6 elements can provide HFR 3D imaging with an acceptable image quality and a corresponding channel count reduction (Fig 1). The image quality degraded for larger MBF sizes. The lateral resolution was 4.6mm and 1mm (same as FSA) at 50mm depth for El and Az direction respectively. The side-lobe levels and CNR in Az was -15dB and 2.2 respectively.

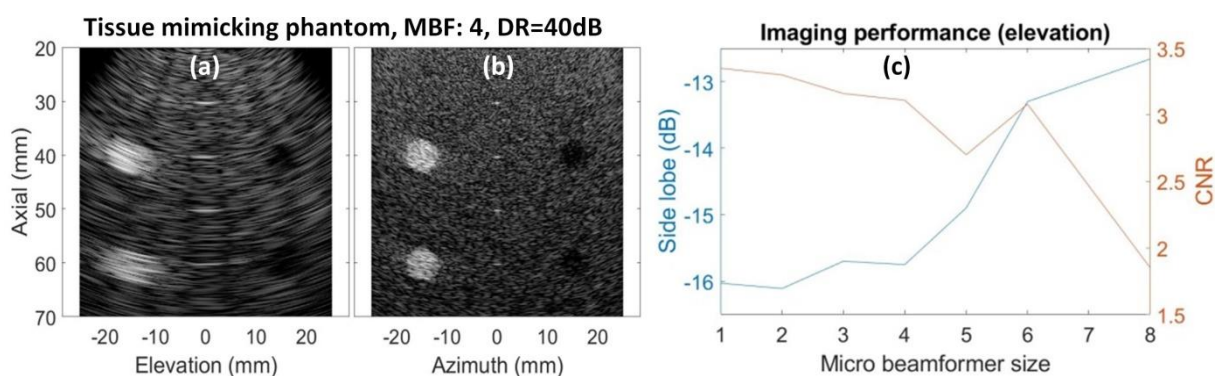


Figure 1. a) A 3D simulated tissue mimicking phantom imaged by the proposed method in elevation and b) in azimuth direction. c) side lobe level and contrast to noise ratio vs. MBF size in elevation